



Asset Criticality Analysis



Contents

Chapter 1: Overview	1
Overview of the Asset Criticality Analysis (ACA) Module	2
Asset Criticality Analysis Workflow	2
Access the ACA Overview Page	2
Access the ACA Overview Page for a Hierarchy Level	3
Chapter 2: Workflow	6
Asset Criticality Analysis: Perform Asset Criticality Analysis Workflow	7
Create Asset Criticality Analysis	7
Assign Assets to Analysis	7
Assess Asset Criticality	7
Approve Analysis	8
Update ABC Indicator in SAP	8
Chapter 3: Asset Criticality Analyses (ACAs)	9
About Asset Criticality Analyses	11
About the Asset Criticality Analysis Team	11
About General Recommendation Records and ACA	11
Access an ACA	12
Access the Analyses Section	12
Create an ACA	13
Access Recommended Actions for an ACA	14
Access the ACA Team Members Section	14
Access the Assets Section	15
Add an Asset	16
Unlink an Asset	17
Apply Assessment to other Assets in Analysis	18
Assess an Asset Via the Risk Matrix	20
Assess an Asset Via the Criticality Checklist	22
View the Revision History of a Criticality Assessment via the Risk Matrix	24

View the Revision History of a Criticality Assessment via the Criticality Checklist	27
Configure ACA Criticality Definition and Checklist Family	30
Send an Asset to a New ACA Analysis	35
Send an Asset to an Existing ACA Analysis	37
Send Assets to an Asset Strategy	39
Send an Asset to a System Strategy	43
Send an Asset to a New FMEA Analysis	45
Send an Asset to an Existing FMEA Analysis	47
Send an Asset to a New RCM Analysis	49
Send an Asset to an Existing RCM Analysis	51
Send an Asset to the RBI Asset View	53
Send an Asset to RBI Asset View from Analysis View	55
Approve an Analysis	55
Update SAP	56
Access Reference Documents for an ACA	58
Export an ACA from Analysis View	58
Export Analyses from the Overview Page	60
Remove an ACA from the ACA Overview Page	60
Chapter 4: Data Loader	62
About the Asset Criticality Analysis (ACA) Data Loader	63
About the Asset Criticality Analysis (ACA) Data Loader Requirements	63
About the Asset Criticality Analysis (ACA) Data Loader Data Model	64
About the Asset Criticality Analysis (ACA Checklist) Data Loader Workbook Layout and Use	64
About the Asset Criticality Analysis (ACA) Data Loader General Loading Strategy	66
About the Asset Criticality Analysis (ACA) Data Loader Workbook Layout and Use	67
About the Asset Criticality Analysis (ACA) Data Loader Load Verification	69
Chapter 5: Deployment	71
Deploy ACA for the First Time	72
Upgrade or Update ACA to V4.4.0.0.0	72
ACA Security Groups	75
Chapter 6: Reference	78

General Reference	79
Family Field Descriptions	82
Catalog Items	86

Copyright GE Digital

© 2020 General Electric Company.

GE, the GE Monogram, and Predix are either registered trademarks or trademarks of All other trademarks are the property of their respective owners.

This document may contain Confidential/Proprietary information of and/or its suppliers or vendors. Distribution or reproduction is prohibited without permission.

THIS DOCUMENT AND ITS CONTENTS ARE PROVIDED "AS IS," WITH NO REPRESENTATION OR WARRANTIES OF ANY KIND, WHETHER EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO WARRANTIES OF DESIGN, MERCHANTABILITY, OR FITNESS FOR A PARTICULAR PURPOSE. ALL OTHER LIABILITY ARISING FROM RELIANCE UPON ANY INFORMATION CONTAINED HEREIN IS EXPRESSLY DISCLAIMED.

Access to and use of the software described in this document is conditioned on acceptance of the End User License Agreement and compliance with its terms.

Chapter 1

Overview

Topics:

- [Overview of the Asset Criticality Analysis \(ACA\) Module](#)
- [Asset Criticality Analysis Workflow](#)
- [Access the ACA Overview Page](#)
- [Access the ACA Overview Page for a Hierarchy Level](#)

Overview of the Asset Criticality Analysis (ACA) Module

Asset Criticality Analysis (ACA) is a tool that you can use to define the criticality assets with APM. The ACA module enables users to define the criticality of assets based on the worst likely case consequence of failure of the asset to provide an overall criticality value. In other words, using an ACA, you can determine which of your systems, locations, and pieces of equipment are critical based on your organizations definition.

After you have determined which of your assets are critical, you can use GE Digital APM modules to further analyze and safeguard those systems, locations, and pieces of equipment. For example, through an ACA, you might discover that if Equipment A were to fail, it could cause a catastrophic event in your facility, leading to personal injury. In this case, Asset A is considered critical, and you may want to use other tools and methodologies with APM to develop a maintenance, inspection or monitoring strategy for optimizing the performance or reliability of Equipment A.

These methodologies could include:

- Reliability Centered Maintenance (RCM)
- Failure Modes and Effects Analysis (FMEA)
- Asset Strategy Management (ASM)
- Risk Based Inspection (RBI)

ACA can leverage either the standard GE Digital APM risk matrix or the combination of a Criticality Checklist and associated Family Policy as the assessment method used for the criticality assessment.

Asset Criticality Analysis Workflow

This topic provides the basic, high-level steps for using ACA. The steps and links in this workflow do not necessarily reference every possible procedure.

1. [Create an Asset Criticality Analysis \(ACA\)](#).
2. [Assign assets to the ACA](#).
3. Assess the criticality of the assets assigned to the ACA [via the Criticality Checklist](#) or [via the Risk Matrix](#).
4. [Approve the ACA](#).
5. [Update SAP](#).

Access the ACA Overview Page

Before You Begin

You can access the **ACA Overview** page only if you are a member of one of the following [Security Groups](#):

- MI ACA Administrator
- MI ACA Member
- MI ACA Owner

About This Task


This topic describes how to access the **ACA Overview** page, on which you can view information and perform various tasks related to **Asset Criticality Analysis** of various Hierarchy Levels. If you want to


view ACAs associated with a particular Hierarchy Level, you can access the **ACA Overview** page for a Hierarchy Level.


You can perform various tasks on this page based on your membership in various Security Groups.

Procedure

In the module navigation menu, select **Strategy > Asset Criticality Analysis**. The **ACA Overview** page appears.

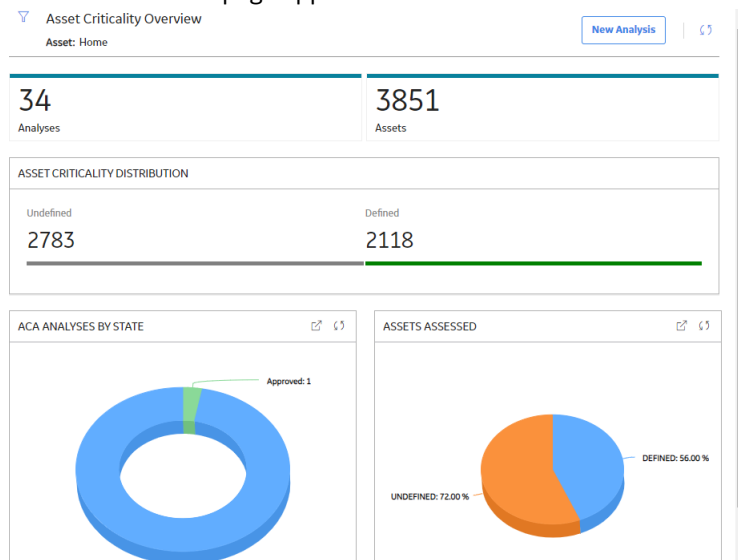

Note: The **Asset Criticality Analysis Overview** page is not updated automatically when you return to the previously opened tab. You can select  to update the page.


By default, the hierarchy level is set to home. You can filter the hierarchy level by selecting  in the page. By default, the ACA information on the page is related to an Asset.

Access the ACA Overview Page for a Hierarchy Level


Before You Begin

- You can access the **ACA Overview** page only if you are a member of one of the following [Security Groups](#):
 - MI ACA Administrator
 - MI ACA Member
 - MI ACA Owner

Procedure

- In the main navigation bar, select . The Asset Hierarchy appears.
- In the **Hierarchy** section, select the asset for which you want to access the analyses. The **<Asset Name>** workspace appears.
- Select the **Strategy** tab.

In the **Strategy** section, you can view module-specific data for the asset, such as strategy actions, recommended actions, ACA analyses, strategies, and so on.

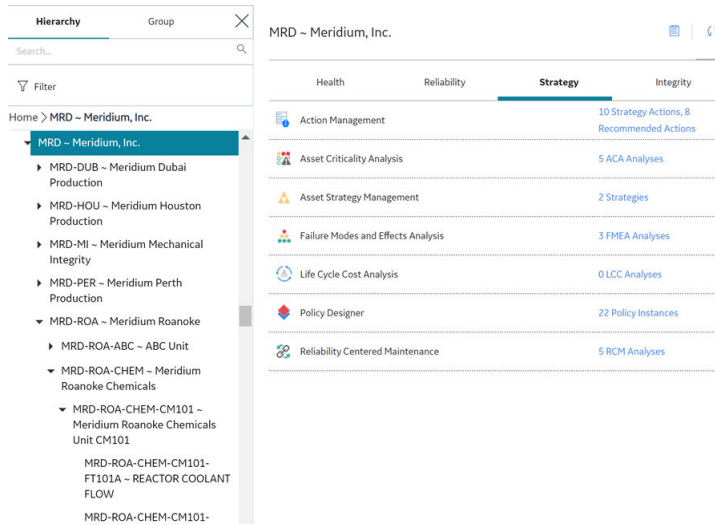


4. In the row containing the number of ACA analyses, select the link.

The **Asset Criticality Overview** page for the selected asset appears, displaying the following information:


- The **Analyses** tab: Select to display a list of all existing ACAs for the selected asset. You can create a new ACA or access an existing one. The number in the **Analyses** tab indicates the number of existing ACA for all users related to the selected asset.
- The **Assets** tab: Select to display a list of the assets based on the asset filter. The number in the **Assets** tab indicates the number of existing assets based on the asset filter.

The workspace displays the following charts that correspond only to the selected hierarchy level:

- **ACA ANALYSES BY STATE:** The chart provides an overview of the number of analyses and the [states of the analyses](#).
- **ASSETS ASSESSED:** Displays the number of pieces of equipment in the database that are ranked based on the risk.

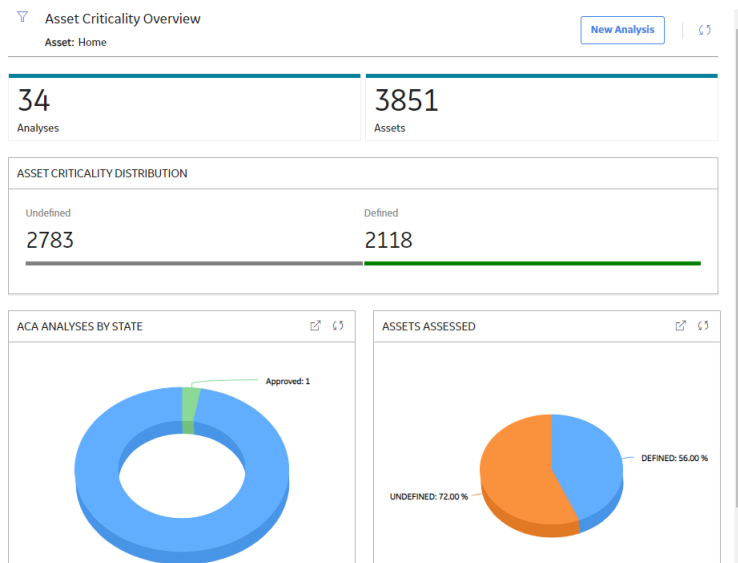

While viewing any of the above charts, you can select  to customize the appearance of the chart.

You can filter the hierarchy level by selecting  in the page. By default, the Asset Criticality Analysis information on the page is related to an asset.

Chapter 2

Workflow


Topics:

- [Asset Criticality Analysis: Perform Asset Criticality Analysis Workflow](#)
- [Create Asset Criticality Analysis](#)
- [Assign Assets to Analysis](#)
- [Assess Asset Criticality](#)
- [Approve Analysis](#)
- [Update ABC Indicator in SAP](#)

Asset Criticality Analysis: Perform Asset Criticality Analysis Workflow

The ACA workflow provides the steps for establishing the criticality of assets with APM. The assessment is based on the worst-likely case consequence of failure of the asset to provide an overall criticality value. This provides a prioritization for asset strategy development, performance improvement efforts and day-to-day asset management activities.

In the following workflow diagram, the blue text in a shape indicates that a corresponding description has been provided in the sections that follow the diagram. For more information, refer to the topic Interpreting the Workflow Diagrams.

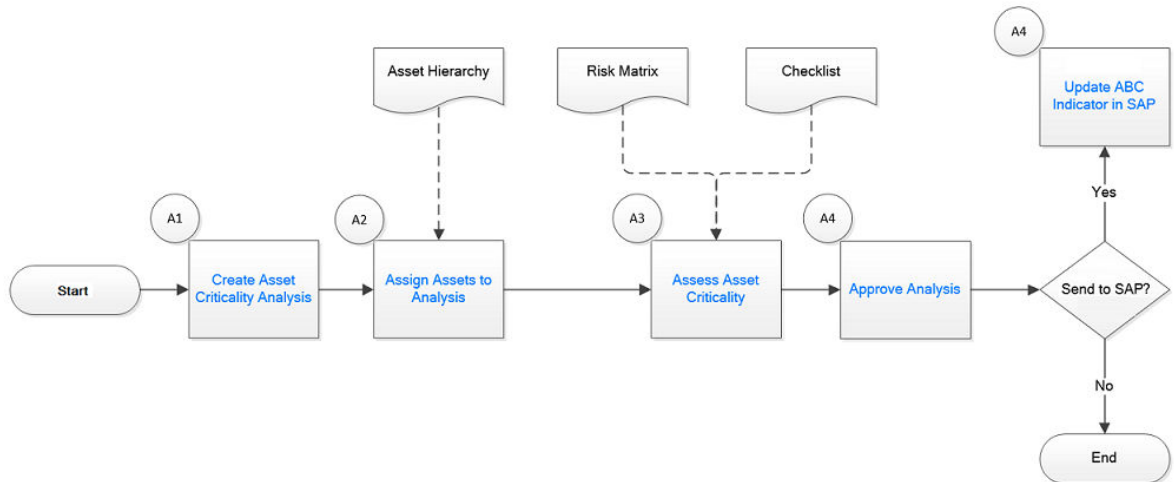

Create Asset Criticality Analysis

Persona: Analyst

Create an Asset Criticality Analysis to assess the criticality of the assets in the analysis.

Assign Assets to Analysis

Persona: Analyst

Assign the assets to an analysis to assess criticality.

Assess Asset Criticality

Persona: Analyst

Assess the criticality of the assets contained in the analysis.

Approve Analysis

Persona: Analyst

Note: The SAP Criticality Interface license is required to approve an analysis.

After the criticality assessments are completed for the assets in an analysis, approve the analysis. Upon approval, the ABC Indicator field for the asset in SAP is automatically updated.

Update ABC Indicator in SAP

Persona: Analyst

Note: The SAP Criticality Interface license is required to perform this operation.

If the send to SAP operation fails, you can manually update the ABC Indicator field for the asset in SAP.

Chapter 3

Asset Criticality Analyses (ACAs)

Topics:

- [About Asset Criticality Analyses](#)
- [About the Asset Criticality Analysis Team](#)
- [About General Recommendation Records and ACA](#)
- [Access an ACA](#)
- [Access the Analyses Section](#)
- [Create an ACA](#)
- [Access Recommended Actions for an ACA](#)
- [Access the ACA Team Members Section](#)
- [Access the Assets Section](#)
- [Add an Asset](#)
- [Unlink an Asset](#)
- [Apply Assessment to other Assets in Analysis](#)
- [Assess an Asset Via the Risk Matrix](#)
- [Assess an Asset Via the Criticality Checklist](#)
- [View the Revision History of a Criticality Assessment via the Risk Matrix](#)
- [View the Revision History of a Criticality Assessment via the Criticality Checklist](#)
- [Configure ACA Criticality Definition and Checklist Family](#)
- [Send an Asset to a New ACA Analysis](#)
- [Send an Asset to an Existing ACA Analysis](#)

- Send Assets to an Asset Strategy
- Send an Asset to a System Strategy
- Send an Asset to a New FMEA Analysis
- Send an Asset to an Existing FMEA Analysis
- Send an Asset to a New RCM Analysis
- Send an Asset to an Existing RCM Analysis
- Send an Asset to the RBI Asset View
- Send an Asset to RBI Asset View from Analysis View
- Approve an Analysis
- Update SAP
- Access Reference Documents for an ACA
- Export an ACA from Analysis View
- Export Analyses from the Overview Page
- Remove an ACA from the ACA Overview Page


About Asset Criticality Analyses

Asset Criticality Analysis (ACA) is a tool that you can use to define the criticality of a system and the individual locations and pieces of equipment that make up that system.

About the Asset Criticality Analysis Team

After you have defined the ACA that you want to conduct, you can define the ACA team by [accessing the ACA Team Members section](#).

After you define the ACA team using these examples, the **Asset Criticality Analysis Team Members** page will look similar to the following image.

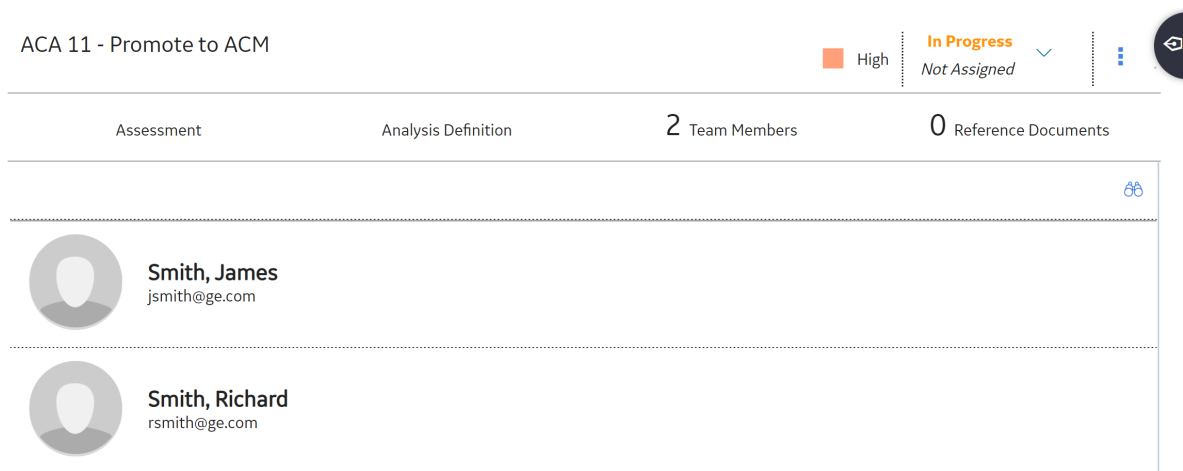


About General Recommendation Records and ACA

At the Analysis level and Asset level, you can add General Recommendation records to the ACA by linking them to [ACA records](#).

If you add to the ACA a record that is already linked to a General Recommendation record, that General Recommendation record will also be added to the ACA automatically.

You will know that a General Recommendation record is linked to an Asset Criticality Analysis System record when you access the **Recommended Actions** pane, which lists the number of Recommended Actions that are currently associated with that system.

For example, the following image shows the grid on the **Asset Criticality Analysis Systems** page. In the **Recommended Actions** column, the text Recommended Actions appears, indicating that the Asset Criticality Analysis System record that appears in that row is linked to one General Recommendation record.

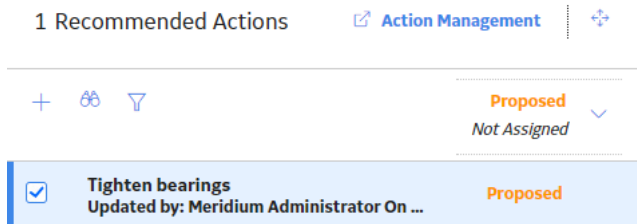

You can manage the General Recommendation records for individual records within an ACA via the **Recommended Actions** pane, or you can view a list of all the General Recommendation records for an ACA via Action Management.

Tip: For information about additional options available when working with the Recommendation records, refer to the Action Management section of the documentation.

Access an ACA

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Analyses** tab.
A grid appears containing a list of ACA analyses.
3. Select the link for the record you want to open.
The **Analysis** workspace appears, displaying the **Assessment** section.

Note: If you want to modify the ACA, select the **Analysis Definition** tab, modify the [available fields](#), and then select  to save your changes.

Access the Analyses Section

Before You Begin

You can access the **ACA Overview** page only if you are a member of one of the following [Security Groups](#):

- MI ACA Administrator
- MI ACA Member
- MI ACA Owner

About This Task

This topic describes how to access the **Analyses** section, in which you can view information and perform various tasks related to analyses of various Asset Hierarchy levels. If you want to view analyses associated with a particular Asset Hierarchy level, you can access the **ACA Overview** page from that Asset Hierarchy level.


Procedure

1. Access the [ACA Overview](#) page.
2. In the **ACA Overview** page, select the **Analyses** tab.
The **Analyses** section appears, displaying a list of available analyses based on the current filter.

Asset Criticality Overview

Asset: Home New Analysis


205	93059																												
Analyses	Assets																												
<table border="1"> <thead> <tr> <th>ANALYSIS</th> <th>STATE</th> <th>STATE ASSIGNEE</th> <th>CRITICALITY ↓</th> </tr> </thead> <tbody> <tr> <td><input type="checkbox"/> Boiler Circulation Pumps</td> <td>In Progress</td> <td></td> <td>Very High</td> </tr> <tr> <td><input type="checkbox"/> Economizer</td> <td>In Progress</td> <td></td> <td>Very High</td> </tr> <tr> <td><input type="checkbox"/> Compressor Criticality</td> <td>In Progress</td> <td></td> <td>Very High</td> </tr> <tr> <td><input type="checkbox"/> Pump criticality</td> <td>In Progress</td> <td></td> <td>Very High</td> </tr> <tr> <td><input type="checkbox"/> Superheater</td> <td>In Progress</td> <td></td> <td>Very High</td> </tr> <tr> <td><input type="checkbox"/> Compressor</td> <td>Approved</td> <td></td> <td>Very High</td> </tr> </tbody> </table>		ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓	<input type="checkbox"/> Boiler Circulation Pumps	In Progress		Very High	<input type="checkbox"/> Economizer	In Progress		Very High	<input type="checkbox"/> Compressor Criticality	In Progress		Very High	<input type="checkbox"/> Pump criticality	In Progress		Very High	<input type="checkbox"/> Superheater	In Progress		Very High	<input type="checkbox"/> Compressor	Approved		Very High
ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓																										
<input type="checkbox"/> Boiler Circulation Pumps	In Progress		Very High																										
<input type="checkbox"/> Economizer	In Progress		Very High																										
<input type="checkbox"/> Compressor Criticality	In Progress		Very High																										
<input type="checkbox"/> Pump criticality	In Progress		Very High																										
<input type="checkbox"/> Superheater	In Progress		Very High																										
<input type="checkbox"/> Compressor	Approved		Very High																										

Note: By default, the Asset Hierarchy level is set to Home. You can modify the Asset Hierarchy level by selecting .

Create an ACA

Procedure

1. Access the [ACA Overview](#) page.
2. Select **New Analysis**.
The **Analysis Definition** workspace appears.

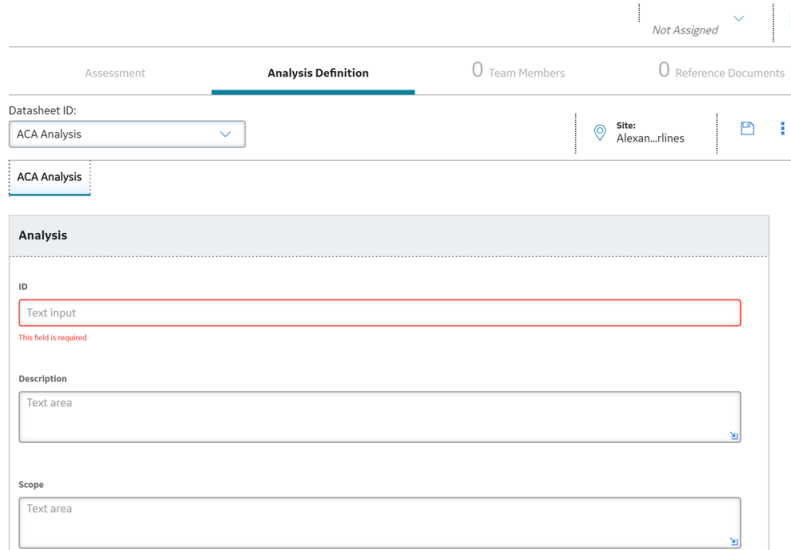


The screenshot shows the 'Analysis Definition' workspace. At the top, there are tabs for 'Assessment', 'Analysis Definition' (selected), 'Team Members', and 'Reference Documents'. The 'Not Assigned' dropdown is visible in the top right. Below the tabs, the 'Datasheet ID' is set to 'ACA Analysis'. The 'Site' is set to 'Alexan...rines'. The main form area is titled 'Analysis' and contains three required fields: 'ID' (Text input), 'Description' (Text area), and 'Scope' (Text area). A red border highlights the 'ID' field, and a red error message 'This field is required' is displayed below it.

3. As needed, enter values in the [available fields](#).
4. In the upper-right corner of the workspace, select **Site**.
Note: By default, the site that the user is assigned to appears.
5. Select the site to which you want to assign the ACA record.

Note: If the ACA record is assigned to the default site, then it can be accessed only by users who have been assigned to the same site. The site selector component becomes read only after it is saved. You will need to log in as a Super User to modify the site. A Super User can change the site to any of the sites that the user has permission for OR choose to make the ACA record as a Global Record by

selecting Global, so that all GE Digital APM users can see it. See the [Site Filtering section of the documentation](#) for more information on using that feature.


6. Select .
The new analysis is saved.


Next Steps

- [Assign assets to the ACA.](#)

Access Recommended Actions for an ACA

Procedure

1. [Access an ACA System.](#)
2. In the workspace, select .
The **Recommended Actions** pane appears, displaying a list of Recommendations associated with that ACA system.

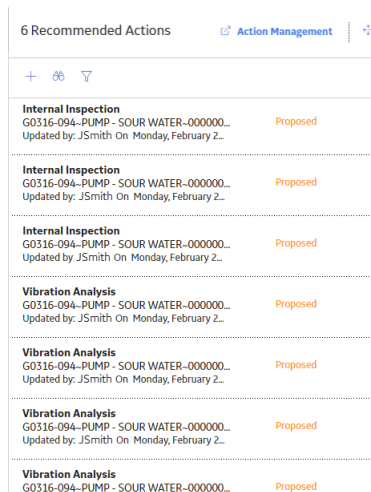

6 Recommended Actions		Action Management
Internal Inspection	G0316-094-PUMP - SOUR WATER-000000...	Proposed
Updated by: JSmith On Monday, February 2...		
Internal Inspection	G0316-094-PUMP - SOUR WATER-000000...	Proposed
Updated by: JSmith On Monday, February 2...		
Internal Inspection	G0316-094-PUMP - SOUR WATER-000000...	Proposed
Updated by: JSmith On Monday, February 2...		
Vibration Analysis	G0316-094-PUMP - SOUR WATER-000000...	Proposed
Updated by: JSmith On Monday, February 2...		
Vibration Analysis	G0316-094-PUMP - SOUR WATER-000000...	Proposed
Updated by: JSmith On Monday, February 2...		
Vibration Analysis	G0316-094-PUMP - SOUR WATER-000000...	Proposed
Updated by: JSmith On Monday, February 2...		
Vibration Analysis	G0316-094-PUMP - SOUR WATER-000000...	Proposed

Note: See the Overview of Recommended Actions section of the documentation for additional options when working with recommendations.

Tip: For information about additional options available when working with the Recommendation records, refer to the Action Management section of the documentation.

Access the ACA Team Members Section

Procedure

1. [Access the ACA](#) for which you want to view team members.
2. Select the **Team Members** tab.
The **Team Members** section appears.



Assessment

Analysis Definition

2 Team Members

0 Reference Documents

Smith, James
jsmith@ge.com

Smith, Richard
rsmith@ge.com

Tip: For details about working with teams and the **Team Members** section, refer to the Teams section of the documentation.

Access the Assets Section

Before You Begin

You can access the **ACA Overview** page only if you are a member of one of the following [Security Groups](#):

- MI ACA Administrator
- MI ACA Member
- MI ACA Owner

About This Task

This topic describes how to access the **Assets** section, in which you can view information and perform tasks related to assets of various Asset Hierarchy levels. If you want to view assets associated with a particular Asset Hierarchy level, you can access the **ACA Overview** page from that Asset Hierarchy level.

Procedure

1. [Access the ACA Overview page.](#)
2. In the **ACA Overview** page, select the **Assets** tab.
The **Assets** section appears, displaying a list of available assets based on the current filter.

Asset Criticality Overview New Analysis

Asset: Home

205


Analyses

93059

Assets

Send To ▾

<input type="checkbox"/> ASSET	ACA	OTHER ANALYSES	STRATEGY
<input type="checkbox"/> MRD ~ ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD ~ ALEXANDERS
<input type="checkbox"/> MRD-ROA-REFN ~ ROANOKE REFINING	A319 Engines	FMEA Analysis	
<input type="checkbox"/> MRD-ROA-REFN-RF002 ~ RF002 - CRUDE	A320 Engines	RCM Analysis	
<input type="checkbox"/> MRD-ROA-REFN-RF004 ~ RF004 - NAPHTHA HYDROTREATER	A320 Engines	FMEA Analysis	
<input type="checkbox"/> MRD-ROA-REFN-RF008 ~ RF008 - COOLING WATER	A321 Engines	FMEA Analysis	
<input type="checkbox"/> MRD-ROA-REFN-RF009 ~ RF009 - STEAM	A350 Engines	FMEA Analysis	


Note: By default, the Asset Hierarchy level is set to home. You can modify the Asset Hierarchy level by selecting .

Add an Asset

This topic lists the steps required to add an asset to an analysis.


Procedure

1. Access the **ACA Overview** page.
2. Select the **Analyses** tab.
The **Analyses** section appears, displaying a list of available analyses based on the current filter.

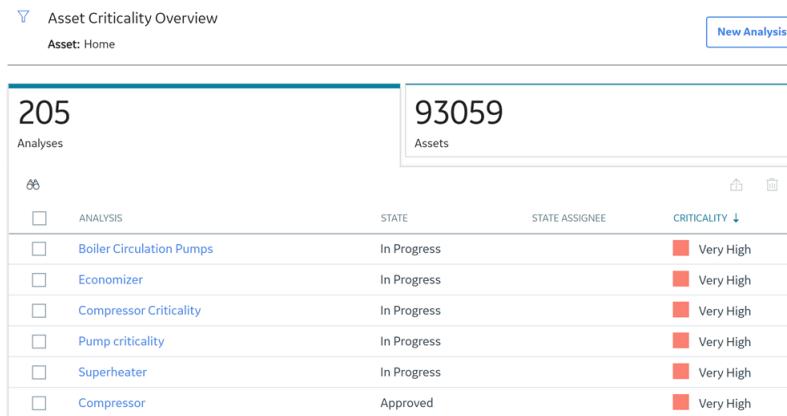

ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓
<input type="checkbox"/> Boiler Circulation Pumps	In Progress		Very High
<input type="checkbox"/> Economizer	In Progress		Very High
<input type="checkbox"/> Compressor Criticality	In Progress		Very High
<input type="checkbox"/> Pump criticality	In Progress		Very High
<input type="checkbox"/> Superheater	In Progress		Very High
<input type="checkbox"/> Compressor	Approved		Very High


3. Select an analysis.
The **Assessment** workspace for the selected analysis appears.

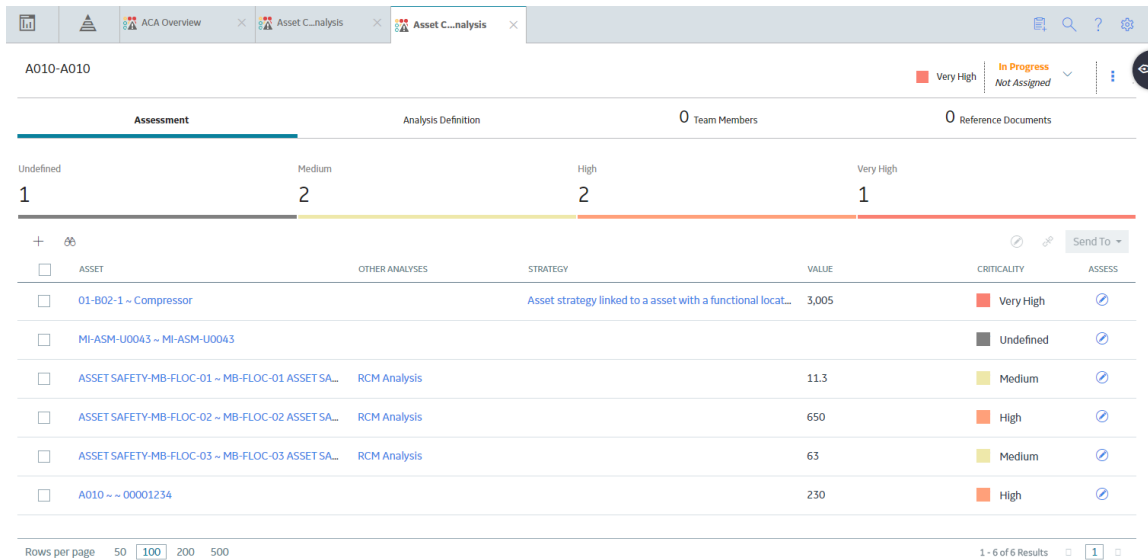

ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
<input type="checkbox"/> 01-B02-1 ~ Compressor		Asset strategy linked to an asset with a functional locat...	3,005	Very High	
<input type="checkbox"/> MI-ASM-U0043 ~ MI-ASM-U0043				Undefined	
<input type="checkbox"/> ASSET SAFETY-MB-FLOC-01 ~ MB-FLOC-01 ASSET SA...	RCM Analysis		11.3	Medium	
<input type="checkbox"/> ASSET SAFETY-MB-FLOC-02 ~ MB-FLOC-02 ASSET SA...	RCM Analysis		650	High	
<input type="checkbox"/> ASSET SAFETY-MB-FLOC-03 ~ MB-FLOC-03 ASSET SA...	RCM Analysis		63	Medium	
<input type="checkbox"/> A010 ~ ~ 00001234			230	High	

4. Select .
- The **Asset Finder** window appears.

Asset Finder

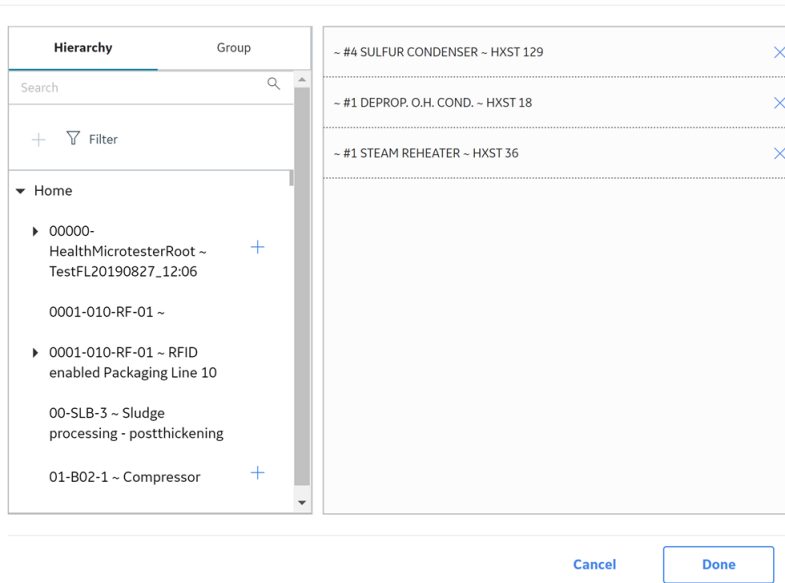

5. In the **Asset Finder** window, make one of the following selections:

Selection	Action
Add a Single Asset	In the Asset Finder window, select the assets you want to link to the analysis, and select + in the row.
Add an Asset Family	In the Asset Finder window, select + next to the Filter button.

The selected assets appear in the right pane of the **Asset Finder** window.

Note: The selected assets must belong to the same site as the current analysis.

6. Select **Done**.
The selected assets are added to the analysis.

Next Steps

Assess the criticality of the assets assigned to the ACA [via the Criticality Checklist](#) or [via the Risk Matrix](#).

Unlink an Asset

This topic lists the steps required to unlink an asset from an analysis.

Procedure

1. [Access the ACA Overview page](#).
2. Select the **Analyses** tab.
The **Analyses** section appears, displaying a list of available analyses based on the current filter.

Asset Criticality Overview

Asset: Home New Analysis

205

Analyses

93059

Assets

	ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓
<input type="checkbox"/>	Boiler Circulation Pumps	In Progress		Very High
<input type="checkbox"/>	Economizer	In Progress		Very High
<input type="checkbox"/>	Compressor Criticality	In Progress		Very High
<input type="checkbox"/>	Pump criticality	In Progress		Very High
<input type="checkbox"/>	Superheater	In Progress		Very High
<input type="checkbox"/>	Compressor	Approved		Very High

- Select an analysis.
The **Assessment** workspace for the selected analysis appears.

A010-A010

Very High In Progress Not Assigned

Assessment Analysis Definition 0 Team Members 0 Reference Documents

Undefined Medium High Very High

1 2 2 1

ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
01-B02-1 - Compressor		Asset strategy linked to an asset with a functional locat...	3,005	Very High	ⓘ
MI-ASM-U0043 - MI-ASM-U0043				Undefined	ⓘ
ASSET SAFETY-MB-FLOC-01 - MB-FLOC-01 ASSET SA...	RCM Analysis		11.3	Medium	ⓘ
ASSET SAFETY-MB-FLOC-02 - MB-FLOC-02 ASSET SA...	RCM Analysis		650	High	ⓘ
ASSET SAFETY-MB-FLOC-03 - MB-FLOC-03 ASSET SA...	RCM Analysis		63	Medium	ⓘ
A010 - ~ 00001234			230	High	ⓘ

Rows per page 50 100 200 500

1 - 6 of 6 Results 1

- Select an asset row.
- Select . A window appears, asking you to confirm that you want to unlink the selected analysis.
- Select **Yes**. The selected assets are unlinked from the analysis.

Apply Assessment to other Assets in Analysis

This topic lists the steps required to apply assessment of an asset to other assets in an analysis.

Procedure

- Access the [ACA Overview](#) page.
- Select the **Analyses** tab.
The **Analyses** section appears, displaying a list of available analyses based on the current filter.

Asset Criticality Overview

Asset: Home New Analysis

205

Analyses

93059

Assets

<input type="checkbox"/>	ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓
<input type="checkbox"/>	Boiler Circulation Pumps	In Progress		Very High
<input type="checkbox"/>	Economizer	In Progress		Very High
<input type="checkbox"/>	Compressor Criticality	In Progress		Very High
<input type="checkbox"/>	Pump criticality	In Progress		Very High
<input type="checkbox"/>	Superheater	In Progress		Very High
<input type="checkbox"/>	Compressor	Approved		Very High

- Select an analysis.
The **Assessment** workspace for the selected analysis appears.

Assessment
Analysis Definition
0 Team Members
0 Reference Documents

Undefined
Medium

3
1

<input type="checkbox"/>	ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
<input type="checkbox"/>	- NO.1 STEAM REHEATER - HXST 152	FMEA Analysis RCM Analysis RBI Asset View	Policy manger test data	65	Medium	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-01 ~ MB-FLOC-01 ASSET ...	RCM Analysis			Undefined	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-02 ~ MB-FLOC-02 ASSET ...	RCM Analysis			Undefined	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-03 ~ MB-FLOC-03 ASSET ...	RCM Analysis			Undefined	

- Select an asset row whose assessment needs to be applied to other assets.
- Select .
The **Apply Assessment To** window appears.



SELECTED ASSESSMENT

~ NO.1 STEAM REHEATER ~ HXST 152 : Medium

APPLY TO



<input type="checkbox"/>	ASSET	ASSIGNED BY	CRITICALITY
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-01 ~ MB-FLO...		Undefined
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-02 ~ MB-FLO...		Undefined
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-03 ~ MB-FLO...		Undefined

Rows per page 50 100 200 500

1 - 3 of 3 Results 1

Cancel

Apply

6. Select the assets on which the same assessment is to be applied and then select **Apply**. The selected assets have the same assessment from the analysis.

Assessment	Analysis Definition	0 Team Members	0 Reference Documents			
Undefined 1	Medium 3					
<input type="checkbox"/>	ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
<input type="checkbox"/>	~ NO.1 STEAM REHEATER ~ HXST 152	FMEA Analysis RCM Analysis RBI Asset View	Policy manger test data	65	Medium	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-01 ~ MB-FLOC-01 ASSET ...	RCM Analysis		65	Medium	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-02 ~ MB-FLOC-02 ASSET ...	RCM Analysis		65	Medium	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-03 ~ MB-FLOC-03 ASSET ...	RCM Analysis			Undefined	

Assess an Asset Via the Risk Matrix

This topic describes how to assess the criticality of an asset with the Risk Matrix. You can also assess asset criticality with the Criticality Checklist.

Before You Begin

There must be an available analysis that contains assets.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Analyses** tab.
The **Analyses** section appears, displaying a list of available analyses based on the current filter.

ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓
<input type="checkbox"/> Boiler Circulation Pumps	In Progress		Very High
<input type="checkbox"/> Economizer	In Progress		Very High
<input type="checkbox"/> Compressor Criticality	In Progress		Very High
<input type="checkbox"/> Pump criticality	In Progress		Very High
<input type="checkbox"/> Superheater	In Progress		Very High
<input type="checkbox"/> Compressor	Approved		Very High

3. Select an analysis.
The **Assessment** section for the selected analysis appears.

ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
<input type="checkbox"/> 01-B02-1 ~ Compressor		Asset strategy linked to an asset with a functional locat...	3,005	Very High	<input checked="" type="checkbox"/>
<input type="checkbox"/> MI-ASM-U0043 ~ MI-ASM-U0043				Undefined	<input checked="" type="checkbox"/>
<input type="checkbox"/> ASSET SAFETY-MB-FLOC-01 ~ MB-FLOC-01 ASSET SA...	RCM Analysis		11.3	Medium	<input checked="" type="checkbox"/>
<input type="checkbox"/> ASSET SAFETY-MB-FLOC-02 ~ MB-FLOC-02 ASSET SA...	RCM Analysis		650	High	<input checked="" type="checkbox"/>
<input type="checkbox"/> ASSET SAFETY-MB-FLOC-03 ~ MB-FLOC-03 ASSET SA...	RCM Analysis		63	Medium	<input checked="" type="checkbox"/>
<input type="checkbox"/> A010 ~ ~ 00001234			230	High	<input checked="" type="checkbox"/>

4. To assess a single asset, next to the asset you want to assess, select .
Note: To assess multiple assets simultaneously, next to each row containing an asset that you want to assess, select the check box, and then select above the grid.

The **Criticality Assessment** section appears.

Criticality Assessment [Revision History](#) ✕

Total Risk

	Probability	Consequence				
		Very Low	Low	Medium	High	Very High
Safety		1	10	100	500	1,000
Environm...	Frequent 5	5	50	500	2,500	5,000
Operations	Probable 1	1	10	100	500	1,000
Financial	Possible 0.3	0.3	3	30	150	300
	Remote 0.1	0.1	1	10	50	100
	Improbable 0.05	0.05	0.5	5	25	50

Not Applicable
 Mitigated Risk:
 Unmitigated Risk

Basis for Assessment

[Cancel](#) [Save](#)

5. Select the appropriate values in the Risk Matrix, and then select **Save**.
The criticality values calculated by the assessment are updated in the grid.

Next Steps

[Approve the ACA.](#)

Assess an Asset Via the Criticality Checklist

This topic describes how to assess the criticality of an asset with the Criticality Checklist. You can also assess asset criticality with the Risk Matrix.

Before You Begin

- There must be an available analysis that contains assets.
- Asset Criticality Analysis must be configured to measure criticality with the Criticality Checklist.

Procedure

1. [Access the ACA Overview page.](#)
2. Select the **Analyses** tab.
The **Analyses** section appears, displaying a list of available analyses based on the current filter.

Asset Criticality Overview

Asset: Home New Analysis

205

Analyses

93059

Assets

<input type="checkbox"/>	ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓
<input type="checkbox"/>	Boiler Circulation Pumps	In Progress		Very High
<input type="checkbox"/>	Economizer	In Progress		Very High
<input type="checkbox"/>	Compressor Criticality	In Progress		Very High
<input type="checkbox"/>	Pump criticality	In Progress		Very High
<input type="checkbox"/>	Superheater	In Progress		Very High
<input type="checkbox"/>	Compressor	Approved		Very High

- Select an analysis. The **Assessment** section for the selected analysis appears.

A010-A010 Very High In Progress Not Assigned

Assessment Analysis Definition 0 Team Members 0 Reference Documents

Undefined	Medium	High	Very High
1	2	2	1

<input type="checkbox"/>	ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
<input type="checkbox"/>	01-B02-1 - Compressor		Asset strategy linked to an asset with a functional locat...	3,005	Very High	
<input type="checkbox"/>	MI-ASM-U0043 - MI-ASM-U0043				Undefined	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-01 - MB-FLOC-01 ASSET SA...	RCM Analysis		11.3	Medium	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-02 - MB-FLOC-02 ASSET SA...	RCM Analysis		650	High	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-03 - MB-FLOC-03 ASSET SA...	RCM Analysis		63	Medium	
<input type="checkbox"/>	A010 - ~ 00001234			230	High	

Rows per page: 50 200 500 1 - 6 of 6 Results

- To assess a single asset, next to the asset you want to assess, select .

Note: To assess multiple assets simultaneously, next to each row containing an asset that you want to assess, select the check box, and then select above the grid.

 The **Criticality Assessment** window appears.

Criticality Assessment [Revision History](#) ✕

Datasheet ID:
 ⋮

Safety Consequence

Environment Consequence

Operations Consequence

PM Required

Basis for Assessment

Assessment: ■ Undefined [Cancel](#)

5. Enter values in the [available fields](#), and then select **Save**.
 The criticality values calculated by the assessment are updated in the grid.

Next Steps

[Approve the ACA.](#)

View the Revision History of a Criticality Assessment via the Risk Matrix

This topic describes how to view the revision history of a criticality assessment for a given asset in the Risk Matrix. You can also view the revision history in the Criticality Checklist.

Before You Begin

There must be an available analysis that contains assets.

Procedure

1. [Access the ACA Overview page.](#)
2. Select the **Analyses** tab.
 The **Analyses** section appears, displaying a list of available analyses based on the current filter.

Asset Criticality Overview

Asset: Home New Analysis

205

Analyses

93059

Assets

<input type="checkbox"/>	ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓
<input type="checkbox"/>	Boiler Circulation Pumps	In Progress		■ Very High
<input type="checkbox"/>	Economizer	In Progress		■ Very High
<input type="checkbox"/>	Compressor Criticality	In Progress		■ Very High
<input type="checkbox"/>	Pump criticality	In Progress		■ Very High
<input type="checkbox"/>	Superheater	In Progress		■ Very High
<input type="checkbox"/>	Compressor	Approved		■ Very High

- Select an analysis. The **Assessment** section for the selected analysis appears.

A010-A010 Very High In Progress Not Assigned

Assessment Analysis Definition 0 Team Members 0 Reference Documents

Undefined 1
Medium 2
High 2
Very High 1

<input type="checkbox"/>	ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
<input type="checkbox"/>	01-B02-1 - Compressor		Asset strategy linked to an asset with a functional locat...	3,005	■ Very High	↻
<input type="checkbox"/>	MI-ASM-U0043 - MI-ASM-U0043				■ Undefined	↻
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-01 - MB-FLOC-01 ASSET SA...	RCM Analysis		11.3	■ Medium	↻
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-02 - MB-FLOC-02 ASSET SA...	RCM Analysis		650	■ High	↻
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-03 - MB-FLOC-03 ASSET SA...	RCM Analysis		63	■ Medium	↻
<input type="checkbox"/>	A010 - ~ 00001234			230	■ High	↻

Rows per page: 50 200 500 1 - 6 of 6 Results

- Select against the asset for which you want to view the revision history. The **Criticality Assessment** section appears.

Total Risk

	Probability	Consequence				
		Very Low	Low	Medium	High	Very High
Safety		1	10	100	500	1,000
Environm...	Frequent 5	5	50	500	2,500	5,000
Operations	Probable 1	1	10	100	500	1,000
Financial	Possible 0.3	0.3	3	30	150	300
	Remote 0.1	0.1	1	10	50	100
	Improbable 0.05	0.05	0.5	5	25	50

Not Applicable
 Mitigated Risk:
 Unmitigated Risk

Basis for Assessment

Cancel

Save

5. Select **Revision History**.

The **Revision History** section for the selected asset appears.

Criticality Assessment ×

[Criticality Assessment for Asset \Revision History\](#)

← Revision History

REVISION DATE/TIME	REVISED BY	BASIS FOR ASSESSMENT	ORIGINAL ASSESSMENT	NEW ASSESSMENT
12/10/2019 16:05:50	Baseline Super User	Steam Reheater test	■ High	■ Medium
12/10/2019 16:03:20	Baseline Super User	Steam Reheater	■ Undefined	■ High

Rows per page: 50 200 500

1 - 2 of 2 Results ← →

6. Select a link in the **REVISION DATE/TIME** column for the record that you want to view.

The revision history of the criticality assessment for the selected asset appear in the grid.

Criticality Assessment ×

... Revision History \12/10/2019 16:05:50\
< Revision History

Total Risk 25

Safety 10	Probability	Consequence				
		Very Low 1	Low 10	Medium 100	High 500	Very High 1,000
Environm... 10	Frequent 5	5	50	500	2,500	5,000
Operations 5	Probable 1	1	10	100	500	1,000
Financial	Possible 0.3	0.3	3	30	150	300
	Remote 0.1	0.1	1	10	50	100
	Improbable 0.05	0.05	0.5	5	25	50

Not Applicable Mitigated Risk: Unmitigated Risk

Basis for Assessment

View the Revision History of a Criticality Assessment via the Criticality Checklist

This topic describes how to view the revision history of a criticality assessment for a given asset in the Criticality Checklist. You can also view the revision history in the Risk Matrix.

Before You Begin

- There must be an available analysis that contains assets.
- Asset Criticality Analysis must be configured to measure criticality with the Criticality Checklist.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Analyses** tab.
The **Analyses** section appears, displaying a list of available analyses based on the current filter.

Asset Criticality Overview

Asset: Home New Analysis

205

Analyses

93059

Assets

<input type="checkbox"/>	ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓
<input type="checkbox"/>	Boiler Circulation Pumps	In Progress		Very High
<input type="checkbox"/>	Economizer	In Progress		Very High
<input type="checkbox"/>	Compressor Criticality	In Progress		Very High
<input type="checkbox"/>	Pump criticality	In Progress		Very High
<input type="checkbox"/>	Superheater	In Progress		Very High
<input type="checkbox"/>	Compressor	Approved		Very High

- Select an analysis.
The **Assessment** section for the selected analysis appears.

A010-A010 Very High In Progress Not Assigned

Assessment Analysis Definition 0 Team Members 0 Reference Documents

Undefined 1
Medium 2
High 2
Very High 1

<input type="checkbox"/>	ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
<input type="checkbox"/>	01-B02-1 - Compressor		Asset strategy linked to an asset with a functional locat...	3,005	Very High	
<input type="checkbox"/>	MI-ASM-U0043 - MI-ASM-U0043				Undefined	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-01 - MB-FLOC-01 ASSET SA...	RCM Analysis		11.3	Medium	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-02 - MB-FLOC-02 ASSET SA...	RCM Analysis		650	High	
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-03 - MB-FLOC-03 ASSET SA...	RCM Analysis		63	Medium	
<input type="checkbox"/>	A010 - ~ 00001234			230	High	

Rows per page 50 100 200 500 1 - 6 of 6 Results 1

- Select against the asset for which you want to view the revision history.
The **Criticality Assessment** section appears.

Criticality Assessment

[Revision History](#) ✕

Datasheet ID:

Criticality Checklist ⌵



Safety Consequence

Environment Consequence

Operations Consequence

PM Required

Basis for Assessment

Text area ⌵

Assessment: ■ Undefined

[Cancel](#)

[Save](#)

5. Select **Revision History**.

The **Revision History** section for the selected asset appears.

Criticality Assessment



[Criticality Assessment for Asset \Revision History\](#)

[←](#) Revision History

🔍

REVISION DATE/TIME	REVISED BY	BASIS FOR ASSESSMENT	ORIGINAL ASSESSMENT	NEW ASSESSMENT
12/10/2019 16:05:50	Baseline Super User	Steam Reheater test	■ High	■ Medium
12/10/2019 16:03:20	Baseline Super User	Steam Reheater	■ Undefined	■ High

Rows per page 50 200 500

1 - 2 of 2 Results ← →

6. Select a link in the **REVISION DATE/TIME** column for the record that you want to view.

The revision history of the criticality assessment for the selected asset appear in the Criticality Checklist datasheet.

Criticality Assessment

... Revision History | 12/10/2019 16:22:57 |

< Revision History

Datasheet ID:
Criticality Checklist

Safety Consequence
LOW

Environment Consequence
LOW

Operations Consequence
LOW

PM Required

Basis for Assessment
Steam Heater Test

Configure ACA Criticality Definition and Checklist Family

This topic provides the steps for configuring ACA Criticality definition and Checklist Family.

1. [Modify or configure a new Criticality Definition](#)
2. [Configure Criticality Thresholds](#)
3. [Configure Criticality Checklist](#)
4. [Configure Family Policy](#)
5. [Configure Criticality Mappings](#)

Modify or Configure a new Criticality Definition

Before You Begin

Associate a Criticality Definition with a Site. If no Site is designated then the Default Criticality Definition will be used.


About This Task


A Default Criticality Definition is provided with the baseline product, additional Criticality Definition records can be added per Site as required.

Procedure


1. Access the Criticality Definition record that you want to associate with a site.
2. In the **Record Explorer** pane, in the Related Families, select **Site Reference**.

Note: If Site Reference does not appear, select , and then select **All Possible Families**.

3. Select , and then select **Link Existing Records**.
The **Search** window appears, displaying a list of entities of the family.
4. In the drop-down list boxes, select the required options to filter the entities from the list.
-or-

In the text box, enter the name of the family or entity that you want to search, and then select 

5. Select the record that you want to link, and then select **OK**.
The records are linked.

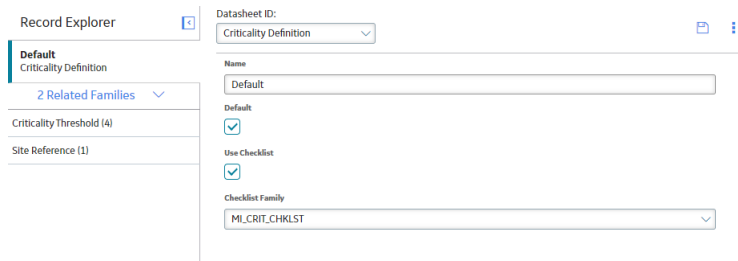

The screenshot shows the 'Record Explorer' window with a 'Criticality Definition' record selected. The 'Name' field is set to 'Default'. The 'Default' checkbox is checked. The 'Use Checklist' checkbox is also checked. The 'Checklist Family' dropdown is set to 'MI_CRIT_CHKLIST'.


Note:

- If the **Use Checklist** check box is not selected, a Risk Matrix will be used for Criticality Assessment for Analyses in the related Site.
- If the **Use Checklist** check box is selected, a Checklist will be used for Criticality Assessment for Analyses in the related Site, and the checklist family to be used must be selected. The MI_CRIT_CHKLIST family is provided with baseline, additional subfamilies can be created to support configuring different checklists per Site.

Configure Criticality Thresholds

About This Task

Criticality Thresholds are provided with the baseline product. These can be modified, or additional Criticality Definition records can be configured per Criticality Definition as required. Each Criticality Threshold has a Description, Value, and Color. The criticality value represents the lowest value in the range for the threshold.

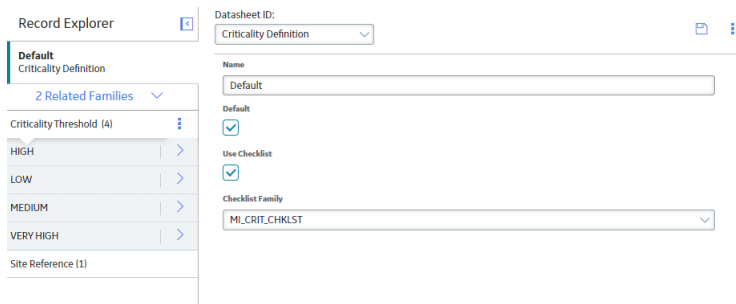

The screenshot shows the 'Record Explorer' window with a 'Criticality Definition' record selected. The 'Name' field is set to 'Default'. The 'Default' checkbox is checked. The 'Use Checklist' checkbox is also checked. The 'Checklist Family' dropdown is set to 'MI_CRIT_CHKLIST'. The 'Criticality Threshold (4)' section is expanded, showing four thresholds: HIGH, LOW, MEDIUM, and VERY HIGH, each with a right-pointing arrow.

Record Explorer

Datasheet ID: Criticality Threshold

Description: High

Value: 100

Color: Light Salmon

2 Related Families

Criticality Threshold (4)

- HIGH
- LOW
- MEDIUM
- VERY HIGH

Site Reference (1)

Configure Criticality Checklist

About This Task

You must configure the fields and behaviors and then configure the datasheet in order to configure the Criticality Checklist. Fields are provided with the baseline product; these fields can be modified, or additional fields can be configured per Criticality Checklist as required.

Entity Relationship

Entity: Criticality Checklist

Last Modified On 4/5/2019 4:21:52 AM Modified By Administrator,Meridium

Information	Fields	Datasheets	Family Reports	Rules and Policies	State Management	Associated Pages
					Field Chooser	+ ◇
ID	CAPTION	DATA TYPE	ACTIVE STATUS	IS IT		
MI_CRIT_CHKLIST_ENVI_CONS_CHR	Environment Consequence	Character	Yes	No		
MI_CRIT_CHKLIST_OPER_CONS_CHR	Operations Consequence	Character	Yes	No		
MI_CRIT_CHKLIST_PM_REQU_FLG	PM Required	Boolean	Yes	No		
MI_CRIT_CHKLIST_CRIT_VALU_NBR	Criticality Value	Numeric	Yes	No		
MI_CRIT_CHKLIST_SAFE_CONS_CHR	Safety Consequence	Character	Yes	No		
MI_CRIT_CHKLIST_BASL_ASSE_TX	Basis for Assessment	Text	Yes	No		

1 - 6 of 6 Results Page 1 of 1

Available Items

Search Fields

Criticality Value

Datasheet Caption: Criticality Checklist

Save

Safety Consequence

Environment Consequence

Operations Consequence

PM Required

Basis for Assessment

Configure Family Policy

Procedure

1. In the module navigation menu, select **Admin > Configuration Manager > Family Management**. The **Family Management** page appears, displaying the list of already existing families. **Home** is selected by default.
2. In the pane, in the **Entity** section, access Criticality Checklist.
3. In the workspace, select the **Rules and Policies** tab.

Entity: Criticality Checklist
Last Modified On 4/5/2019 4:21:52 AM Modified By Administrator,Meridium

Information Fields Datasheets Family Reports **Rules and Policies** State Management Associated Pages

None VB Rules Family Policies

Before Insert	Edit
After Insert	Add
Before Update	Add
After Update	Add
Before Delete	Add
After Delete	Add

4. Select **Edit** corresponding to the **Before Insert** option. The **Design** workspace appears.

Details Design

Inputs Conditions Logic Calculations Actions Edit Save

n3 - Properties

Name: SAF

Output Type: Integer

Input Value: Current Entity

Safety Consequence

Note: The **Before Insert Family Policy** is used to calculate the criticality value that will be saved to Criticality Family that gets translated to Criticality Threshold.

5. Select **Save**. A Family Policy is configured.

Configure Criticality Mappings

Criticality mapping in ACA can optionally be configured if you are using SAP Criticality Assessment Interface.

About This Task

In SAP systems, each Equipment and Functional Location contains a criticality indicator value. If you have a SAP system and your ACA Analyses include Equipment and Functional Location records that were created from SAP (using the SAP interfaces), when you assess criticality in ACA, you can also update the corresponding criticality indicator values in SAP with the ACA values.

To enable this functionality, you must first create Criticality Mapping records, which identify the criticality indicator values in your SAP system (e.g., A, B, C). You will need to link each Criticality Mapping record to the Criticality Threshold record that represents the APM criticality value that should be mapped to the SAP criticality indicator values (e.g., High, Medium, Low). If you are using multiple SAP Systems, you can link one Criticality Mapping record for each system to the same Criticality Threshold record.

To create a Criticality Mapping record and link it to a Criticality Threshold record:

Procedure

1. Access the Criticality Definition datasheet of the record that is used by your ACA Analyses.
2. In the **Record Explorer** pane, expand the **Criticality Threshold** node.
3. Expand the node of the Criticality Threshold record for which you want to map criticality values (i.e., High, Low, Medium, or Very High).
4. Right-click the **Criticality Mapping** family node, and then select **Create a New Criticality Mapping to link to <Criticality Threshold record>**.
A new **Criticality Mapping** record appears.

The screenshot shows the SAP Criticality Assessment Interface. On the left is the 'Record Explorer' pane with a tree view containing 'Default Criticality Definition', 'HIGH Criticality Threshold', 'PRF-800 - A - Prod. loss involved Criticality Mapping', 'All Possible Families', 'Criticality Threshold (0)', and 'Risk Threshold (0)'. The main area displays the 'Criticality Mapping' form. At the top, 'Datasheet ID' is set to 'Criticality Mapping'. Below this, there are three dropdown menus: 'Values(s)', 'CMMS ID' (selected as 'PRF-800'), and 'Indicator' (selected as 'A - Prod. loss involved').

5. In the **CMMS ID** list, select the SAP system to which you want to transfer criticality values. This list displays the value in the **System ID** field for each SAP System record in GE Digital APM.
6. In the **Indicator** list, select the SAP criticality indicator value to which you want to map the criticality threshold that is represented by the criticality threshold record to which this Criticality Mapping record is linked.
The list displays the criticality indicator values in the SAP system that you selected.
7. Select **OK**.
8. Repeat steps 3 through 7 for each Criticality Threshold record defined for your Criticality Definition.
9. Select **Save**.
The new Criticality Mapping record is linked to the selected Criticality Threshold record.

Send an Asset to a New ACA Analysis

This topic provides the steps for sending an asset to a new ACA Analysis.

Procedure

1. Access the [ACA Overview](#) page.

2. Select the **Assets** tab.

The **Assets** section appears, displaying a list of available assets based on the current filter.

The screenshot shows the 'Asset Criticality Overview' page. At the top, there is a breadcrumb 'Asset: Home' and a 'New Analysis' button. Below this, there are two tabs: 'Analyses' (with a count of 205) and 'Assets' (with a count of 93059). The 'Assets' tab is active, displaying a table with columns for 'ASSET', 'ACA', 'OTHER ANALYSES', and 'STRATEGY'. A 'Send To' dropdown menu is visible in the top right of the table area. The first row of the table is highlighted.

<input type="checkbox"/>	ASSET	ACA	OTHER ANALYSES	STRATEGY
<input type="checkbox"/>	MRD - ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD - ALEXANDERS
<input type="checkbox"/>	MRD-ROA-REFN - ROANOKE REFINING	A319 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF002 - RF002 - CRUDE	A320 Engines	RCM Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF004 - RF004 - NAPHTHA HYDROTREATER	A320 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF008 - RF008 - COOLING WATER	A321 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF009 - RF009 - STEAM	A350 Engines	FMEA Analysis	

3. In the **Assets** section, select the check box in the row containing the asset you want to send to a new ACA Analysis.
The asset is highlighted.

Asset Criticality Overview
Asset: Home

New Analysis

33 Analyses

3727 Assets

Send To

(14)	ASSET	ACA	OTHER ANALYSES	STRATEGY	CRITICALITY
<input type="checkbox"/>	19-00400 SOUR WATER		FMEA Analysis	19-00400	Undefined
<input type="checkbox"/>	0001-001-01 Test1				Undefined
<input type="checkbox"/>	QA Test Piping Circuit			QA Test Piping Circuit	Undefined
<input checked="" type="checkbox"/>	AQA 50 TMLs				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-01				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-02				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-03				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-04				Undefined
<input checked="" type="checkbox"/>	AQA Auto Piping Circuit ...				Undefined
<input checked="" type="checkbox"/>	QA Piping Circuit with S...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - In...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - O...				Undefined
<input checked="" type="checkbox"/>	QA PV Cylindrical Shell -...				Undefined

Rows per page 50 100 200 500

1 - 100 of 3727 Results

- In the section, select the **Send To** drop-down menu, and select **ACA Analysis**.
- In the **Send to ACA Analysis** window, if it is not already selected, select **Create New**. The window displays options for you to create a new ACA Analysis.

Send to ACA Analysis

Link Existing Create New

Datasheet ID:
Asset Criticality

Site:
Roan..., VA

Main Log

System ID:
Text input
This field is required

System Description:
Text area

Site ID:

Cancel Send

- Complete the required fields, and select **Send**. Your asset is sent to a new ACA Analysis and will be connected to the ACA analysis when the linking process completes.

Note:

- The **Send To Status** process indicator appears in the workspace. When the process is completed, a notification appears.
- Upon successful completion, a link to the ACA Analysis appears in the **ACA** column for the asset.

Send an Asset to an Existing ACA Analysis

This topic provides the steps for sending an asset to an existing ACA Analysis.

Procedure

1. Access the **ACA Overview** page.
2. Select the **Assets** tab.
The **Assets** section appears, displaying a list of available assets based on the current filter.

Asset Criticality Overview
Asset: Home New Analysis

205 Analyses | 93059 Assets

<input type="checkbox"/>	ASSET	ACA	OTHER ANALYSES	STRATEGY	Send To ▾
<input type="checkbox"/>	MRD ~ ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD ~ ALEXANDERS	
<input type="checkbox"/>	MRD-ROA-REFN ~ ROANOKE REFINING	A319 Engines	FMEA Analysis		
<input type="checkbox"/>	MRD-ROA-REFN-RF002 ~ RF002 - CRUDE	A320 Engines	RCM Analysis		
<input type="checkbox"/>	MRD-ROA-REFN-RF004 ~ RF004 - NAPHTHA HYDROTREATER	A320 Engines	FMEA Analysis		
<input type="checkbox"/>	MRD-ROA-REFN-RF008 ~ RF008 - COOLING WATER	A321 Engines	FMEA Analysis		
<input type="checkbox"/>	MRD-ROA-REFN-RF009 ~ RF009 - STEAM	A350 Engines	FMEA Analysis		

3. In the **Assets** section, select the check box in the row containing the asset you want to send to an existing ACA Analysis.
The asset is highlighted.

Asset Criticality Overview

Asset: Home

New Analysis

33 Analyses

3727 Assets

Send To

(14)	ASSET	ACA	OTHER ANALYSES	STRATEGY	CRITICALITY
<input type="checkbox"/>	19-00400 SOUR WATER		FMEA Analysis	19-00400	Undefined
<input type="checkbox"/>	0001-001-01 Test1				Undefined
<input type="checkbox"/>	QA Test Piping Circuit			QA Test Piping Circuit	Undefined
<input checked="" type="checkbox"/>	AQA 50 TMLs				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-01				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-02				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-03				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-04				Undefined
<input checked="" type="checkbox"/>	AQA Auto Piping Circuit ...				Undefined
<input checked="" type="checkbox"/>	QA Piping Circuit with S...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - In...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - O...				Undefined
<input checked="" type="checkbox"/>	QA PV Cylindrical Shell -...				Undefined

Rows per page 50 100 200 500

1 - 100 of 3727 Results

Note: If an ACA is listed in the **ACA** column, you cannot send it to another ACA.

- In the section, select the **Send To** drop-down menu, and select **ACA Analysis**. A window appears, displaying a list of existing analyses that you can send to.

Send to ACA Analysis

Link Existing Create New

ID

ACA-11-Promote to ASM-Node-01

Analysis_v3.4.0-System_V3.4.0

ASF Asset Criticality Analysis-ASF Asset Criticality Analysis System

A001-A001

A002-A002

A010-A010

A11-A11

Multiple Systems-System Node-01

1 - 18 of 18 Results

Page 1 of 1

Cancel Send

- Select the System ID for an analysis, and select **Send**.

The asset is sent to an existing ACA Analysis and will be connected to the ACA Analysis when the sending process completes.

Note:

- The **Send To Status** process indicator appears in the workspace. When the process completes, a notification appears.
- Upon successful completion, a hyperlink to the ACA Analysis appears in the **ACA** column for the asset.

Send Assets to an Asset Strategy

This topic provides the steps for sending assets to an Asset Strategy or sending assets to an Asset Strategy and applying an Asset Strategy Template.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Assets** tab.

The **Assets** section appears, displaying a list of available assets based on the current filter.

Asset Criticality Overview
Asset: Home New Analysis

205 Analyses		93059 Assets		
ASSET	ACA	OTHER ANALYSES	STRATEGY	
<input type="checkbox"/> MRD ~ ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD ~ ALEXANDERS	
<input type="checkbox"/> MRD-ROA-REFN ~ ROANOKE REFINING	A319 Engines	FMEA Analysis		
<input type="checkbox"/> MRD-ROA-REFN-RF002 ~ RF002 - CRUDE	A320 Engines	RCM Analysis		
<input type="checkbox"/> MRD-ROA-REFN-RF004 ~ RF004 - NAPHTHA HYDROTREATER	A320 Engines	FMEA Analysis		
<input type="checkbox"/> MRD-ROA-REFN-RF008 ~ RF008 - COOLING WATER	A321 Engines	FMEA Analysis		
<input type="checkbox"/> MRD-ROA-REFN-RF009 ~ RF009 - STEAM	A350 Engines	FMEA Analysis		

3. In the **Assets** section, select the check boxes against the rows containing the assets that you want to send to an Asset Strategy.
The selected assets are highlighted.

33 Analyses		3727 Assets			
					Send To ▾
<input checked="" type="checkbox"/> (14)	ASSET	ACA	OTHER ANALYSES	STRATEGY	CRITICALITY
<input type="checkbox"/>	19-00400 SOUR WATER		FMEA Analysis	19-00400	Undefined
<input type="checkbox"/>	0001-001-01 Test1				Undefined
<input type="checkbox"/>	QA Test Piping Circuit			QA Test Piping Circuit	Undefined
<input checked="" type="checkbox"/>	AQA 50 TMLs				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-01				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-02				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-03				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-04				Undefined
<input checked="" type="checkbox"/>	AQA Auto Piping Circuit ...				Undefined
<input checked="" type="checkbox"/>	QA Piping Circuit with S...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - In...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - O...				Undefined
<input checked="" type="checkbox"/>	QA PV Cylindrical Shell -...				Undefined

Rows per page 50 200 500

1 - 100 of 3727 Results ← 2 3 4 5 ... 38 →

Note: You cannot send assets for which a strategy is already listed in the **Strategy** column to a different asset strategy.

4. Select **Send To**, and then select **Asset Strategy**. The **Send to Asset Strategy** window appears.

Send to Asset Strategy✕

Create Strategy Create Strategy From Template

A Strategy will be created for the following assets:

- AQA 50 TMLs
- AQA-10TMLS-01
- AQA-10TMLS-02
- AQA-10TMLS-03
- AQA-10TMLS-04
- AQA Auto Piping Circuit 1 For Automation
- QA PV Pipe Nozzle
- QA PV Hemispherical Head - Outside
- QA PV Hemispherical Head - Inside
- QA PV Cylindrical Shell - Outside
- QA PV Cylindrical Shell - Inside
- QA PV Conical Head - Outside
- QA PV Conical Head - Inside
- QA Piping Circuit with Subcomponents

Cancel Create

5. To create an asset strategy for the selected assets, select **Create**.
An Asset Strategy is created and the selected assets are sent to the Asset Strategy. The assets are connected to the Asset Strategy when the process is completed.
Note:
 - The status of the process can be viewed from the **Send To Status** process indicator.
 - Upon successful completion, a link to the Asset Strategy appears in the **Strategy** column for the asset.
6. To apply an Asset Strategy Template when creating an asset strategy for the selected assets, perform the following steps:
 - a) Select the option **Create Strategy From Template**.
The **Select a Template** section appears.

Send to Asset Strategy ×

Create Strategy
 Create Strategy From Template

Select a Template
Application Method
Confirmation

ID	CRITICALITY	DUTY	SERVICE	DESCRIPTION	MILSM_STATE_ID_C	LAST_UPDT_DT
A12					Active	09/30/2013 15:07:30
A13					Active	09/30/2013 15:18:53
ASI AIR COOLER				ASI AIR COOLER Strate...	Active	05/31/2008 02:07:29
ASI Bearing				ASI Bearing Strategy i...	Active	05/31/2008 02:08:15
ASI Power Supply				ASI AIR COOLER Strate...	Active	05/31/2008 02:07:55
ASI Switch				Strategy imported fro...	Active	05/31/2008 02:05:56
ASI tank				Strategy imported fro...	Active	06/03/2008 01:47:31
ASO Small					Active	05/18/2011 00:06:47
Asset strategy linked t...				Asset strategy linked t...	Active	05/19/2010 21:44:33
Asset strategy with up...				Asset strategy with up...	Active	07/02/2008 18:35:57

1 - 35 of 35 Results ← Page 1 of 1 →

Next

- b) Select a template that you want to apply and select **Next**.
The **Application Method** section appears.

Send to Asset Strategy ×

Create Strategy
 Create Strategy From Template

Select a Template
Application Method
Confirmation

Select to apply the template as a copy or as a master:

Apply the template as a copy
 Apply the template as a master

Select which portions of the template to apply

Apply both actions and risks
 Apply risks only

Select how existing items should be handled in existing Asset Strategies

Mark existing items for deletion
 Append the template items to the existing items

Previous
Next

- c) Select the application method and select **Next**.
The **Confirmation** section appears.

Send to Asset Strategy ✕

Create Strategy
 Create Strategy From Template

Select a Template
Application Method
Confirmation

A Strategy will be created for the following assets using Actions and Risks from Strategy Template - ASO Small Existing Items will be marked for deletion

- QA 50 TMLs
- QA-10TMLS-01
- QA-10TMLS-02
- QA-10TMLS-03
- QA-10TMLS-04
- QA Auto Piping Circuit 1 For Automation
- QA Piping Circuit with Subcomponents
- QA PV Conical Head - Inside
- QA PV Conical Head - Outside
- QA PV Cylindrical Shell - Inside
- QA PV Cylindrical Shell - Outside
- QA PV Hemispherical Head - Inside
- QA PV Hemispherical Head - Outside
- QA PV Pipe Nozzle

An Asset Strategy is created and the selected assets are sent to the Asset Strategy. The Asset Strategy Template is applied and the assets are connected to the Asset Strategy when the process is completed.

Note:

- The status of the process can be viewed from the **Send To Status** process indicator.
- Upon successful completion, a link to the Asset Strategy appears in the **Strategy** column for the asset.

Send an Asset to a System Strategy

This topic provides the steps for sending an asset to a System Strategy.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Assets** tab.
The **Assets** section appears, displaying a list of available assets based on the current filter.

Asset Criticality Overview

Asset: Home

205 Analyses		93059 Assets		
ASSET	ACA	OTHER ANALYSES	STRATEGY	Send To
<input type="checkbox"/> MRD - ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD - ALEXANDERS	
<input type="checkbox"/> MRD-ROA-REFN - ROANOKE REFINING	A319 Engines	FMEA Analysis		
<input type="checkbox"/> MRD-ROA-REFN-RF002 - RF002 - CRUDE	A320 Engines	RCM Analysis		
<input type="checkbox"/> MRD-ROA-REFN-RF004 - RF004 - NAPTHA HYDROTREATER	A320 Engines	FMEA Analysis		
<input type="checkbox"/> MRD-ROA-REFN-RF008 - RF008 - COOLING WATER	A321 Engines	FMEA Analysis		
<input type="checkbox"/> MRD-ROA-REFN-RF009 - RF009 - STEAM	A350 Engines	FMEA Analysis		

3. In the **Assets** section, select the check box in the row containing the asset you want to send to a System Strategy.

The asset is highlighted.

Asset Criticality Overview

Asset: Home New Analysis

33 Analyses 3727 Assets

Send To

(14)	ASSET	ACA	OTHER ANALYSES	STRATEGY	CRITICALITY
<input type="checkbox"/>	19-00400 SOUR WATER		FMEA Analysis	19-00400	Undefined
<input type="checkbox"/>	0001-001-01 Test1				Undefined
<input type="checkbox"/>	QA Test Piping Circuit			QA Test Piping Circuit	Undefined
<input checked="" type="checkbox"/>	AQA 50 TMLs				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-01				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-02				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-03				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-04				Undefined
<input checked="" type="checkbox"/>	AQA Auto Piping Circuit ...				Undefined
<input checked="" type="checkbox"/>	QA Piping Circuit with S...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - In...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - O...				Undefined
<input checked="" type="checkbox"/>	QA PV Cylindrical Shell -...				Undefined

Rows per page 50 200 500 1 - 100 of 3727 Results 1 2 3 4 5 ... 38

Note: If a strategy is listed in the **Strategy** column, you cannot send it to another strategy.

- In the section, select the **Send To** drop-down menu, and select **System Strategy**. A window appears.

Send to System Strategy

Are you sure you want to create a System Strategy and Asset Strategy for the selected asset(s)?

- Select **Yes**. The asset is sent to a new System Strategy and will be connected to the System Strategy when the sending process completes.

Note:

- The **Send To Status** process indicator appears in the workspace. When the process completes, a notification appears.
- Upon successful completion, a hyperlink to the System Strategy appears in the **Strategy** column for the asset.

Send an Asset to a New FMEA Analysis

This topic provides the steps for sending an asset to a new FMEA Analysis.

Procedure

1. Access the [ACA Overview](#) page.

2. Select the **Assets** tab.

The **Assets** section appears, displaying a list of available assets based on the current filter.

The screenshot shows the 'Asset Criticality Overview' page. At the top, there is a navigation bar with 'Asset: Home' and a 'New Analysis' button. Below this, there are two main sections: 'Analyses' (with a count of 205) and 'Assets' (with a count of 93059). The 'Assets' section contains a table with columns for 'ASSET', 'ACA', 'OTHER ANALYSES', and 'STRATEGY'. A 'Send To' dropdown menu is visible in the top right of the table. The first row of the table is highlighted.

<input type="checkbox"/>	ASSET	ACA	OTHER ANALYSES	STRATEGY
<input type="checkbox"/>	MRD - ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD - ALEXANDERS
<input type="checkbox"/>	MRD-ROA-REFN - ROANOKE REFINING	A319 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF002 - RF002 - CRUDE	A320 Engines	RCM Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF004 - RF004 - NAPHTHA HYDROTREATER	A320 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF008 - RF008 - COOLING WATER	A321 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF009 - RF009 - STEAM	A350 Engines	FMEA Analysis	

3. In the **Assets** section, select the check box in the row containing the asset you want to send to a new FMEA Analysis.
The asset is highlighted.

33 Analyses		3727 Assets			
					Send To ▾
<input type="checkbox"/> (14)	ASSET	ACA	OTHER ANALYSES	STRATEGY	CRITICALITY
<input type="checkbox"/>	19-00400 SOUR WATER		FMEA Analysis	19-00400	Undefined
<input type="checkbox"/>	0001-001-01 Test1				Undefined
<input type="checkbox"/>	QA Test Piping Circuit			QA Test Piping Circuit	Undefined
<input checked="" type="checkbox"/>	AQA 50 TMLs				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-01				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-02				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-03				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-04				Undefined
<input checked="" type="checkbox"/>	AQA Auto Piping Circuit ...				Undefined
<input checked="" type="checkbox"/>	QA Piping Circuit with S...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - In...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - O...				Undefined
<input checked="" type="checkbox"/>	QA PV Cylindrical Shell -...				Undefined

Rows per page 50 200 500

1 - 100 of 3727 Results ← 2 3 4 5 ... 38 →

Note: If an FMEA Analysis is listed in the **Other Analyses** column, you cannot send it to another FMEA Analysis.

- In the section, select the **Send To** drop-down menu, and select **FMEA Analysis**.
- In the **Send to FMEA Analysis** window, if it is not already selected, select **Create New**. A window appears, allowing you to create a new FMEA Analysis.

Send to FMEA Analysis
✕

Link Existing
 Create New

Datasheet ID:

Analysis

Site: Roan..., VA

Analysis Identification

System Definition

⋮

Value(s)

Analysis ID

745

Analysis Short Description

Text input

This field is required

Analysis Long Description

Text area

Cancel

Send

6. Complete the required fields, and select **Send**.
The asset is sent to a new FMEA Analysis and will be connected to the FMEA analysis when the sending process completes.

Note:

- The **Send To Status** process indicator appears in the workspace. When the process completes, a notification appears.
- Upon successful completion, a hyperlink to the FMEA Analysis appears in the **Other Analyses** column for the asset.

Send an Asset to an Existing FMEA Analysis

This topic provides the steps for sending an asset to an existing FMEA Analysis.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Assets** tab.
The **Assets** section appears, displaying a list of available assets based on the current filter.

Asset Criticality Overview New Analysis

Asset: Home

205

Analyses

93059

Assets

Send To ▾

	ASSET	ACA	OTHER ANALYSES	STRATEGY
<input type="checkbox"/>	MRD ~ ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD ~ ALEXANDERS
<input type="checkbox"/>	MRD-ROA-REFN ~ ROANOKE REFINING	A319 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF002 ~ RF002 - CRUDE	A320 Engines	RCM Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF004 ~ RF004 - NAPTHA HYDROTREATER	A320 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF008 ~ RF008 - COOLING WATER	A321 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF009 ~ RF009 - STEAM	A350 Engines	FMEA Analysis	

- In the **Assets** section, select the check box in the row containing the asset you want to send to an existing FMEA Analysis. The asset is highlighted.

Asset Criticality Overview New Analysis

Asset: Home

33

Analyses

3727

Assets

Send To ▾

	ASSET	ACA	OTHER ANALYSES	STRATEGY	CRITICALITY
<input type="checkbox"/>	19-00400 SOUR WATER		FMEA Analysis	19-00400	Undefined
<input type="checkbox"/>	0001-001-01 Test1				Undefined
<input type="checkbox"/>	QA Test Piping Circuit			QA Test Piping Circuit	Undefined
<input checked="" type="checkbox"/>	AQA 50 TMLs				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-01				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-02				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-03				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-04				Undefined
<input checked="" type="checkbox"/>	AQA Auto Piping Circuit ...				Undefined
<input checked="" type="checkbox"/>	QA Piping Circuit with S...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - In...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - O...				Undefined
<input checked="" type="checkbox"/>	QA PV Cylindrical Shell -...				Undefined

Rows per page 50 100 200 500
 1 - 100 of 3727 Results

Note: If an FMEA Analysis is listed in the **Other Analyses** column, you cannot send it to another FMEA Analysis.

- In the section, select the **Send To** drop-down menu, and select **FMEA Analysis**. A window appears, displaying a list of existing analyses that you can send to.

Send to FMEA Analysis
✕

Link Existing
 Create New

⌕

ANALYSIS ID	ANALYSIS SHORT DESCRIPTION
46	Cooling Tower - Recommendation to Task Mapping
49	Cooling Tower - Task ID Relationship
63	Linked Equipment Analysis 63
67	Event-Based Evaluation
68	Complete Analysis 68
86	Event-Based Evaluation - Failure Count
87	Event-Based Evaluation - Failure Cost
88	Risk Assessment QA Analysis

1 - 46 of 46 Results
← Page 1 of 1 →

Cancel

Send

5. Select an Analysis ID, and select **Send**.

The asset is sent to the existing FMEA Analysis and will be connected to the FMEA analysis when the sending process completes.

Note:

- The **Send To Status** process indicator appears in the workspace. When the process completes, a notification appears.
- Upon successful completion, a hyperlink to the FMEA Analysis appears in the **Other Analyses** column for the asset.

Send an Asset to a New RCM Analysis

This topic provides the steps for sending an asset to a new RCM Analysis.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Assets** tab.
The **Assets** section appears, displaying a list of available assets based on the current filter.

Asset Criticality Overview New Analysis

Asset: Home

205

Analyses

93059

Assets

	ASSET	ACA	OTHER ANALYSES	STRATEGY
<input type="checkbox"/>	MRD ~ ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD ~ ALEXANDERS
<input type="checkbox"/>	MRD-ROA-REFN ~ ROANOKE REFINING	A319 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF002 ~ RF002 - CRUDE	A320 Engines	RCM Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF004 ~ RF004 - NAPTHA HYDROTREATER	A320 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF008 ~ RF008 - COOLING WATER	A321 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF009 ~ RF009 - STEAM	A350 Engines	FMEA Analysis	

- In the **Assets** section, select the check box in the row containing the asset you want to send to a new RCM Analysis. The asset is highlighted.

Asset Criticality Overview New Analysis

Asset: Home

33

Analyses

3727

Assets

	ASSET	ACA	OTHER ANALYSES	STRATEGY	CRITICALITY
<input type="checkbox"/>	19-00400 SOUR WATER		FMEA Analysis	19-00400	Undefined
<input type="checkbox"/>	0001-001-01 Test1				Undefined
<input type="checkbox"/>	QA Test Piping Circuit			QA Test Piping Circuit	Undefined
<input checked="" type="checkbox"/>	AQA 50 TMLs				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-01				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-02				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-03				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-04				Undefined
<input checked="" type="checkbox"/>	AQA Auto Piping Circuit ...				Undefined
<input checked="" type="checkbox"/>	QA Piping Circuit with S...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - In...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - O...				Undefined
<input checked="" type="checkbox"/>	QA PV Cylindrical Shell -...				Undefined

Rows per page: 50 100 200 500 1 - 100 of 3727 Results

Note: If an RCM Analysis is listed in the **Other Analyses** column, you cannot send it to another RCM Analysis.

- In the section, select the **Send To** drop-down menu, and select **RCM Analysis**.
- In the Send to RCM Analysis window, if it is not already selected, select **Create New**. A window appears, allowing you to create a new RCM Analysis.

Send to RCM Analysis ✕

Link Existing
 Create New

Datasheet ID: Site: Roan..., VA

Analysis ⋮

Analysis Identification System Definition ⋮

Value(s)

Analysis ID

804

Analysis Short Description

Text input

This field is required

Analysis Long Description

Text area

Cancel
Send

6. Complete the required fields, and select **Send**.
The asset is sent to a new RCM Analysis and will be connected to the RCM analysis when the sending process completes.

Note:

- The **Send To Status** process indicator appears in the workspace. When the process completes, a notification appears.
- Upon successful completion, a hyperlink to the RCM Analysis appears in the **Other Analyses** column for the asset.

Send an Asset to an Existing RCM Analysis

This topic provides the steps for sending an asset to an existing RCM Analysis.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Assets** tab.
The **Assets** section appears, displaying a list of available assets based on the current filter.

Asset Criticality Overview New Analysis

Asset: Home

205

Analyses

93059

Assets

Send To ▾

	ASSET	ACA	OTHER ANALYSES	STRATEGY
<input type="checkbox"/>	MRD ~ ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD ~ ALEXANDERS
<input type="checkbox"/>	MRD-ROA-REFN ~ ROANOKE REFINING	A319 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF002 ~ RF002 - CRUDE	A320 Engines	RCM Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF004 ~ RF004 - NAPTHA HYDROTREATER	A320 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF008 ~ RF008 - COOLING WATER	A321 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF009 ~ RF009 - STEAM	A350 Engines	FMEA Analysis	

- In the **Assets** section, select the check box in the row containing the asset you want to send to an existing RCM Analysis. The asset is highlighted.

Asset Criticality Overview New Analysis

Asset: Home

33

Analyses

3727

Assets

Send To ▾

	ASSET	ACA	OTHER ANALYSES	STRATEGY	CRITICALITY
<input type="checkbox"/>	19-00400 SOUR WATER		FMEA Analysis	19-00400	Undefined
<input type="checkbox"/>	0001-001-01 Test1				Undefined
<input type="checkbox"/>	QA Test Piping Circuit			QA Test Piping Circuit	Undefined
<input checked="" type="checkbox"/>	AQA 50 TMLs				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-01				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-02				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-03				Undefined
<input checked="" type="checkbox"/>	AQA-10TMLs-04				Undefined
<input checked="" type="checkbox"/>	AQA Auto Piping Circuit ...				Undefined
<input checked="" type="checkbox"/>	QA Piping Circuit with S...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - In...				Undefined
<input checked="" type="checkbox"/>	QA PV Conical Head - O...				Undefined
<input checked="" type="checkbox"/>	QA PV Cylindrical Shell -...				Undefined

Rows per page 50 100 200 500
 1 - 100 of 3727 Results

Note: If an RCM Analysis is listed in the **Other Analyses** column, you cannot send it to another RCM Analysis.

- In the section, select the **Send To** drop-down menu, and select **RCM Analysis**. A window appears, displaying a list of existing analyses that you can send to.

Send to RCM Analysis ×

Link Existing
 Create New

🔍

ANALYSIS ID	ANALYSIS SHORT DESCRIPTION
34	Outlet 234 - Recommendation Bundling
35	Cent Pump 17 - Review Recommendation
38	Cooling Tower - Recommendation to Task Mapping
40	Cooling Tower - Task ID Relationship
59	Linked Equipment Analysis 59
60	Link Equipment(s) Analysis 60
71	Event-Based Evaluation
84	Event-Based Evaluation - Failure Count

1 - 41 of 41 Results ← Page 1 of 1 →

Cancel
Send

5. Select an Analysis ID, and select **Send**.

Note:

- A **Send To Status** process indicator appears in the workspace. When the process completes, a notification appears.
- Upon successful completion, a hyperlink to the RCM Analysis appears in the **Other Analyses** column for the asset.

Send an Asset to the RBI Asset View

This topic provides the steps for sending an asset to an RBI Asset View.

Before You Begin

An asset must be a functional equipment asset to be sent to the RBI Asset View.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Assets** tab.
The **Assets** section appears, displaying a list of available assets based on the current filter.

Asset Criticality Overview
Asset: Home New Analysis

205

Analyses

93059

Assets

	ASSET	ACA	OTHER ANALYSES	STRATEGY
<input type="checkbox"/>	MRD ~ ALEXANDERSON CORPORATION	A320 Engines	FMEA Analysis	MRD ~ ALEXANDERS
<input type="checkbox"/>	MRD-ROA-REFN ~ ROANOKE REFINING	A319 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF002 ~ RF002 - CRUDE	A320 Engines	RCM Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF004 ~ RF004 - NAPTHA HYDROTREATER	A320 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF008 ~ RF008 - COOLING WATER	A321 Engines	FMEA Analysis	
<input type="checkbox"/>	MRD-ROA-REFN-RF009 ~ RF009 - STEAM	A350 Engines	FMEA Analysis	

- In the **Assets** section, select the check box in the row containing the asset you want to send to an RBI Asset View.
The asset is highlighted.

Note: If an RBI Asset View is listed, you cannot view the asset in RBI Asset View.

Asset Criticality Overview
Asset: Home New Analysis

46

Analyses

2789

Assets

	ASSET	ACA	
<input type="checkbox"/>	RBIT-UNIT-A ~ RBIT-UNIT-A		Analysis_v3.4.0-System_V3.4.0
<input type="checkbox"/>	RBIT-UNIT-B ~ RBIT-UNIT-B		
<input type="checkbox"/>	RBIT-UNIT-C ~ RBIT-UNIT-C		
<input type="checkbox"/>	RBIT-UNIT-D ~ RBIT-UNIT-D		
<input type="checkbox"/>	MRD-ROA-REFN-RF104-GBT0001-104 ~ TURBINE - FORCED DRAFT NORTH BOILER STEAM		
<input type="checkbox"/>	GBT0001-104 ~ STEAM TURBINE - 2116GBT0001 ~ 000000000001061286		
<input type="checkbox"/>	-- V350 QA RBI Equ w PRD Component		
<input type="checkbox"/>	-- V350 QA RBI Equ w PRD Asset		
<input checked="" type="checkbox"/>	-- RBI EQU COMP ALL DATA		Multiple Systems-System Node-03
<input type="checkbox"/>	-- RBI EQU NO COMP		

- In the section, select the **Send To** drop-down menu, and select **RBI Asset View**.
A new section appears, displaying the Asset Summary of the asset.

Asset Summary

~ C-488 LUBE/SEAL OIL COO...

Asset: ~ C-488 LUBE/SEAL OIL COOLER ~ HXST 105

Inspection Plan (Proposed)

Cylindrical Shell ~ HXST 105

Asset Overview
Asset Details

Components
■ What-If Risk Analysis

Send an Asset to RBI Asset View from Analysis View


This topic provides the steps for sending an asset to an RBI Asset View.

Before You Begin

An asset must be a functional equipment asset to be sent to the RBI Asset View.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Analyses** tab.
A grid appears which contains a list of ACA analyses.
3. Select the link for the analysis you would like to open.
The **Analysis** workspace for the analysis you selected appears, displaying the **Assessment** section.
4. In the **Assessment** section, select the check box in the row containing the asset you want to send to an RBI Asset View.
The asset is highlighted.
5. Select the **Send To** drop-down menu, and select **RBI Asset View**.
A new section appears, displaying the Asset Summary of the asset.

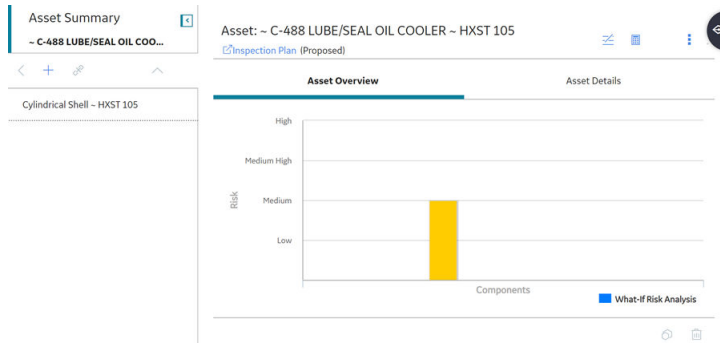

Approve an Analysis

This topic provides the steps to approve an analysis.

Before You Begin

You can access the **ACA Overview** page only if you are a member of one of the following [Security Groups](#):

- MI ACA Administrator
- MI ACA Member
- MI ACA Owner

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Analyses** tab.
The **Analyses** section appears, displaying a list of available analyses based on the current filter.

205	93059		
Analyses	Assets		
<input type="checkbox"/> ANALYSIS STATE STATE ASSIGNEE CRITICALITY ↓			
<input type="checkbox"/>	Boiler Circulation Pumps	In Progress	Very High
<input type="checkbox"/>	Economizer	In Progress	Very High
<input type="checkbox"/>	Compressor Criticality	In Progress	Very High
<input type="checkbox"/>	Pump criticality	In Progress	Very High
<input type="checkbox"/>	Superheater	In Progress	Very High
<input type="checkbox"/>	Compressor	Approved	Very High

- Select the analysis you want to approve. The **Assessment** section appears.
- Select the State Configuration button.
- Select **Approve**.
- Select **Done**. A window appears.

Approve

Are you sure you want to perform the Approve operation?

Yes
No

- Select **Yes**. The analysis is moved to the Approved state.

Next Steps

[Update SAP.](#)

Update SAP

This topic describes how to update SAP from the Analysis View.

Procedure

- Access the [ACA Overview](#) page.
- Select the **Analyses** tab. The **Analyses** section appears, displaying a list of available analyses based on the current filter.

Asset Criticality Overview

Asset: Home New Analysis

205

Analyses

93059

Assets

<input type="checkbox"/>	ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓
<input type="checkbox"/>	Boiler Circulation Pumps	In Progress		Very High
<input type="checkbox"/>	Economizer	In Progress		Very High
<input type="checkbox"/>	Compressor Criticality	In Progress		Very High
<input type="checkbox"/>	Pump criticality	In Progress		Very High
<input type="checkbox"/>	Superheater	In Progress		Very High
<input type="checkbox"/>	Compressor	Approved		Very High

- Select an analysis. The **Assessment** section for the selected analysis appears.

A010-A010 Very High In Progress Not Assigned

Assessment Analysis Definition 0 Team Members 0 Reference Documents

Undefined	Medium	High	Very High
1	2	2	1

<input type="checkbox"/>	ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
<input type="checkbox"/>	01-B02-1 - Compressor		Asset strategy linked to an asset with a functional locat...	3,005	Very High	ⓘ
<input type="checkbox"/>	MI-ASM-U0043 - MI-ASM-U0043				Undefined	ⓘ
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-01 - MB-FLOC-01 ASSET SA...	RCM Analysis		11.3	Medium	ⓘ
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-02 - MB-FLOC-02 ASSET SA...	RCM Analysis		650	High	ⓘ
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-03 - MB-FLOC-03 ASSET SA...	RCM Analysis		63	Medium	ⓘ
<input type="checkbox"/>	A010 - ~ 00001234			230	High	ⓘ

Rows per page: 50 100 200 500 1 - 6 of 6 Results

- Select , and then select **Update SAP**. A window appears, asking you to confirm that you want to update SAP.
- Select **Yes**. SAP is updated.

Note: When the process is completed, you can select the completion date or the **View Error Logs** link to view the status and the status message in the **Update SAP Logs** page.

Update SAP Logs

ASSET	STATUS	MESSAGE
00000000011048706	Success	Successfully sent to the EAM System

Rows per page 50 200 500

1 - 1 of 1 Results ← →

Close

Access Reference Documents for an ACA

Procedure

1. [Access an ACA](#).
2. Select the **Reference Documents** tab.
The **Reference Documents** section appears, displaying the list of available reference documents.

~ NO.1 STEAM REHEATER ~ HXST 152 -ACA analysis-SYstem for ~ NO.1 STE... Undefined In Progress Not Assigned

Assessment	Analysis Definition	0 Team Members	3 Reference Documents	
< + 🔗 🔄			🔗 🗑️	
ID	DESCRIPTION	LAST UPDATED BY	LAST UPDATED DATE	
<input type="checkbox"/> Download JPG	Download JPG	admin , unifiedqa	11/15/2019	
<input type="checkbox"/> Download png	Download png	admin , unifiedqa	11/15/2019	
<input type="checkbox"/> Download TIFF	Download TIFF	admin , unifiedqa	11/15/2019	

Rows per page 50 200 500 1 - 3 of 3 Results ← →

Tip: For more information, refer to the Reference Documents section of the documentation.

Export an ACA from Analysis View

Procedure

1. [Access the ACA Overview](#) page.
2. Select the **Analyses** tab.
The **Analyses** section appears, displaying a list of available analyses based on the current filter.

Asset Criticality Overview

Asset: Home New Analysis

205

Analyses

93059

Assets

<input type="checkbox"/>	ANALYSIS	STATE	STATE ASSIGNEE	CRITICALITY ↓
<input type="checkbox"/>	Boiler Circulation Pumps	In Progress		Very High
<input type="checkbox"/>	Economizer	In Progress		Very High
<input type="checkbox"/>	Compressor Criticality	In Progress		Very High
<input type="checkbox"/>	Pump criticality	In Progress		Very High
<input type="checkbox"/>	Superheater	In Progress		Very High
<input type="checkbox"/>	Compressor	Approved		Very High

- Select an analysis.
The **Assessment** workspace for the selected analysis appears.

A010-A010 Very High In Progress Not Assigned

Assessment
Analysis Definition
0 Team Members
0 Reference Documents

Undefined	Medium	High	Very High
1	2	2	1

<input type="checkbox"/>	ASSET	OTHER ANALYSES	STRATEGY	VALUE	CRITICALITY	ASSESS
<input type="checkbox"/>	01-B02-1 - Compressor		Asset strategy linked to a asset with a functional locat...	3,005	Very High	<input type="checkbox"/>
<input type="checkbox"/>	MI-ASM-U0043 - MI-ASM-U0043				Undefined	<input type="checkbox"/>
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-01 - MB-FLOC-01 ASSET SA...	RCM Analysis		11.3	Medium	<input type="checkbox"/>
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-02 - MB-FLOC-02 ASSET SA...	RCM Analysis		650	High	<input type="checkbox"/>
<input type="checkbox"/>	ASSET SAFETY-MB-FLOC-03 - MB-FLOC-03 ASSET SA...	RCM Analysis		63	Medium	<input type="checkbox"/>
<input type="checkbox"/>	A010 - ~ 00001234			230	High	<input type="checkbox"/>

Rows per page: 50 200 500 1 - 6 of 6 Results

- Select , and select **Export**.
The **Export to a File** window appears.

Export to a File

Please provide a File Name

Cancel


Export

- In the **Please provide a File Name** box, enter a file name for the export.
- Select **Export**.
The selected analysis is exported and appears in an Excel document.

Export Analyses from the Overview Page

This topic describes how to export analyses.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Analyses** tab.
The **Analyses** section appears.
3. Next to each analysis that you want to export, select the check box.
4. Select .
The **Export to a File** window appears.

Export to a File

Please provide a File Name

CancelExport

5. In the **Please provide a File Name** box, enter a file name for the export.
6. Select **Export**.
The selected analyses are exported to an Excel document.


Remove an ACA from the ACA Overview Page

About This Task

You can remove an ACA record from the **ACA Overview** page using . When you remove an ACA record:

- The record is removed from the **ACA Overview** page.
- The links between that record and the other records associated with the ACA are deleted.

Procedure

1. Access the [ACA Overview](#) page.
2. Select the **Analyses** tab.
A grid appears, which contains all of the available ACA records.
3. Select the row for the record that you want to remove, and select .
The ACA record is removed.

Note: Though the record is removed from the **ACA Overview** page, it can still be accessed on the GE Digital APM database in the search results under the name of the record itself, or a search under Asset Criticality Analysis.

Chapter 4

Data Loader

Topics:

- [About the Asset Criticality Analysis \(ACA\) Data Loader](#)
- [About the Asset Criticality Analysis \(ACA\) Data Loader Requirements](#)
- [About the Asset Criticality Analysis \(ACA\) Data Loader Data Model](#)
- [About the Asset Criticality Analysis \(ACA Checklist\) Data Loader Workbook Layout and Use](#)
- [About the Asset Criticality Analysis \(ACA\) Data Loader General Loading Strategy](#)
- [About the Asset Criticality Analysis \(ACA\) Data Loader Workbook Layout and Use](#)
- [About the Asset Criticality Analysis \(ACA\) Data Loader Load Verification](#)

About the Asset Criticality Analysis (ACA) Data Loader

The ACA Data Loader allows existing or new Asset Criticality Analyses to be delivered to the ACA module in GE Digital APM for further development, analysis or implementation. Customers will be able to load data from other external systems into the ACA module via the Excel workbook. They will be able to upload any existing analyses with updated risk assessment data that has been assessed outside the GE Digital APM application. Sites assignments for the ACA records that are loaded with the ACA Data Loader are inherited from the related Assets that already exist in the GE Digital APM system.

The ACA Data Loader is used in the following scenarios:

- Users conducting an initial data load of Asset Criticality Analyses containing Assets for the purpose of completing Criticality Assessments inside the GE Digital APM application.
- Users updating existing Asset Criticality Analyses with Criticality Assessments completed outside the GE Digital APM application.

The ACA module contains two data loaders. To determine which ACA Data Loader to use:

- Use the **Asset Criticality Analysis (ACA) Data Loader** if the Risk Matrix is your Criticality Assessment input method.
- Use the **Asset Criticality Analysis (ACA Checklist) Data Loader** if the Criticality Checklist is your Criticality Assessment input method.

Note: If you are using an export file generated from a version of GE Digital APM prior to V4.3.0.7, then that Excel file needs to be modified to match the current ACA Data Loader template.

About the Asset Criticality Analysis (ACA) Data Loader Requirements

To use the ACA Data Loader, your organization must have completed the deployment of the Asset Criticality Analysis module. The ACA Data Loader should only be used after the Asset Criticality Analysis module has been implemented, and you have defined Assets for your organization.

Mapping

The ACA Data Loader maps the datasheet columns in the Excel workbook to fields in GE Digital APM families. As a minimum, the standard worksheets contain columns that match all fields in standard ACA datasheets.

Mapping exists for all standard family fields, if you have added custom fields to a family, you must ensure that mappings exist for those fields, or data may not be populated as expected following the data load. If you have a custom risk matrix, you must modify the data load worksheet to reflect the risk categories and risk values appropriate for your risk matrix.

If you have a custom risk matrix, you must modify the data load worksheet to reflect the risk categories and risk values appropriate for your risk matrix.


Security Settings

The Security User performing the data load operation must be associated with either the MI Data Loader User or MI Data Loader Admin Security Role, and must also be associated with the MI ACA Administrator Security Group or a Security Role that is associated with this Security Group

About the Asset Criticality Analysis (ACA) Data Loader Data Model

The data for an ACA Analysis is loaded from a single Excel workbook `Asset Criticality Analysis (ACA) .xlsx` containing multiple worksheets. This includes Analysis, Asset and Criticality Assessment data. These elements are highlighted with a red box around the relevant functional areas from the ACA data model extract shown below. Elements shown without a red border are data model elements that will not need to be loaded by the data loader. If using a Criticality Checklist, the data for an ACA Analysis is loaded from a single Excel workbook `Asset Criticality Analysis (ACA Checklist) .xlsx` containing multiple worksheets.

Note: Asset Group is created internally and is not loaded by the data loader.

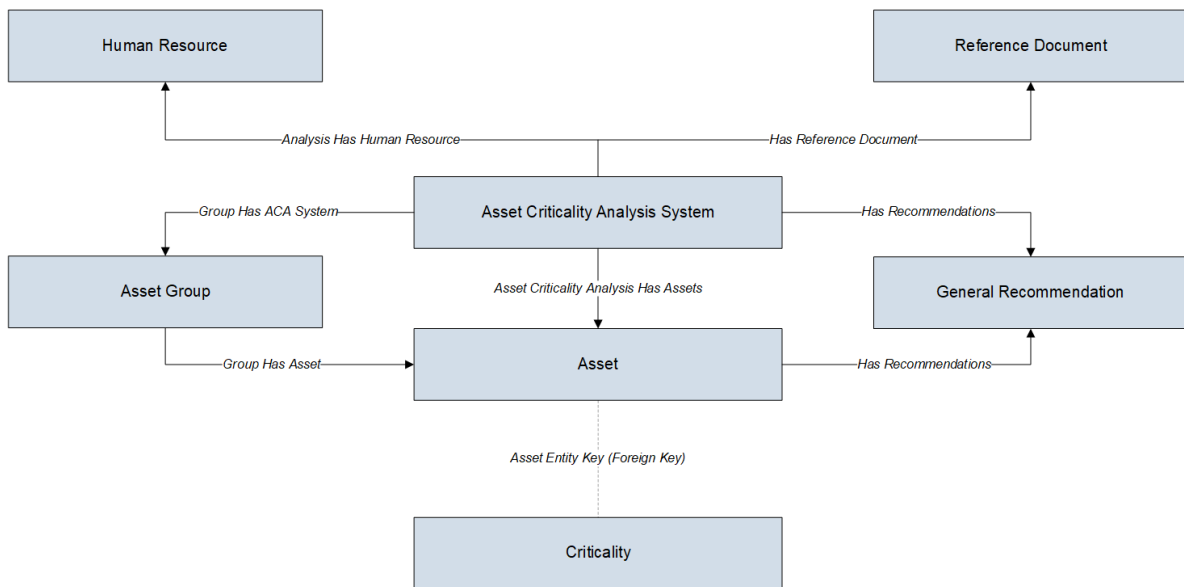

About the Asset Criticality Analysis (ACA Checklist) Data Loader Workbook Layout and Use

This section provides a high-level overview and explanation of how the data loader workbook is constructed if using the Checklist to assess criticality.

In order to import data using the ACA Data Loader, GE Digital APM provides an Excel workbook, `Asset Criticality Analysis (ACA Checklist) .xlsx`, which supports baseline Asset Criticality Analysis in GE Digital APM. This workbook must be used to perform the data load. You can modify the Excel template to include custom fields used by your organization.

The master Excel workbook contains one worksheet for each node that will be populated in the data model.

The following table lists the worksheets that are included in the **Asset Criticality Analysis (ACA Checklist)** workbook.

Worksheet Description

Worksheet	Description
Analysis	This worksheet is used to specify data for import to the Asset Criticality Analysis System family.
Asset	This worksheet is used to specify data for import as Assets related to the ACA Analysis as well as criticality assessment data for each asset.

Each worksheet in the ACA Data Loader Template workbook contains field values that must be mapped to the appropriate GE Digital APM family/field combination. The individual sections in this document specify the source and target fields and relationships required between predecessor and successor.

The list of fields tabulated is not exhaustive. The user can add additional field columns to the worksheets and still perform a successful upload, provided:

- Column fields are properly mapped within the worksheet
- Equivalent fields exist in ACA

Analysis Worksheet

On the Analysis worksheet, you will specify the Analysis ID to which you want to link the Assets. The Analysis ID column that appears on this worksheet also appear on the Assets worksheet, and is used to identify the records that will be linked to the analysis.

Note: Each row in this worksheet represents a unique analysis. You should not include the same analysis more than once.

Field Caption	Field ID	Data Type (Length)	Comments
Site Name	MI_SITE_NAME	Character (255)	This field is required and must be unique.
System Description	MI_ASCRTSYS_SYSTEM_DESCR _T	Text	A brief description of the analysis.
System ID	MI_ASCRTSYS_SYSTEM_ID_C	Character (50)	This field is required and must match an existing Site name. Note: If you want to set the site reference to be a Global Site Reference, enter the constant '*Global*' in the MI_SITE_NAME column on the spreadsheet.

Asset Worksheet

On the Asset worksheet, you will specify the assets that will be created and linked to an analysis.

Note: Each row in this worksheet represents a unique Asset. You should not include the same asset more than once to the same analysis.

Field Caption	Field ID	Data Type (Length)	Comments
Asset ID	ASSET_ID	Character (255)	This field displays the value that identifies the asset.
Asset Field ID	ASSET_FIELD_ID	Character (255)	This field displays the identification of the field of an asset.
Asset Family ID	ASSET_FAMILY	Character (255)	This field is populated automatically.
Basis for Assessment	MI_CRIT_CHKLIST_BASI_ASSE_T X	Text	This field is populated based on the Criticality Checklist of the Site.
Environment Consequence	MI_CRIT_CHKLIST_ENVI_CONS_ CHR	Numeric	This field is populated based on the Criticality Checklist of the Site.
Operations Consequence	MI_CRIT_CHKLIST_OPER_CONS_ CHR	Numeric	This field is populated based on the Criticality Checklist of the Site.
Safety Consequence	MI_CRIT_CHKLIST_SAFE_CONS_ SHR	Numeric	This field is populated based on the Criticality Checklist of the Site.
System ID	MI_ASCRTSYS_SYSTEM_ID_C	Character (255)	The System ID must be unique with respect to other systems that belong to the same analysis.

About the Asset Criticality Analysis (ACA) Data Loader General Loading Strategy

This section describes any prerequisites to loading the data and the order in which the data will be loaded.

Note: Before reading this section, refer to the [Data Model](#) section.

Prerequisite

- The sites to which ACA records are to be assigned have been created.

Load Sequence

Note: If you want to set the site reference to be a Global Site Reference, enter the constant '*Global*' in the MI_SITE_NAME column on the spreadsheet.

The ACA data load must be performed in a specific sequence to successfully populate fields, create records and link them to the predecessor and/or successor records:

1. Create the ACA Analysis.
2. Create and link one or more Assets to the ACA Analysis through the Asset Criticality Analysis Has Assets relationship.

3. Create Criticality records by populating the fields for the Risk Matrix associated with the Site of the Asset. If using a criticality Checklist, then you will create criticality records by populating the fields for the Checklist associated with the Site of the Asset.

About the Asset Criticality Analysis (ACA) Data Loader Workbook Layout and Use

This section provides a high-level overview and explanation of how the data loader workbook is constructed if using the Risk Matrix to assess criticality.

In order to import data using the ACA Data Loader, GE Digital APM provides an Excel workbook, `Asset Criticality Analysis (ACA).xlsx`, which supports baseline Asset Criticality Analysis in GE Digital APM. This workbook must be used to perform the data load. You can modify the Excel template to include custom fields used by your organization.

The master Excel workbook contains one worksheet for each node that will be populated in the data model.

The following table lists the worksheets that are included in the **Asset Criticality Analysis (ACA)** workbook.

Worksheet	Description
Analysis	This worksheet is used to specify data for import to the Asset Criticality Analysis System family.
Asset	This worksheet is used to specify data for import as Assets related to the ACA Analysis as well as criticality assessment data for each asset.

Each worksheet in the ACA Data Loader Template workbook contains field values that must be mapped to the appropriate GE Digital APM family/field combination. The individual sections in this document specify the source and target fields and relationships required between predecessor and successor.

The list of fields tabulated is not exhaustive. The user can add additional field columns to the worksheets and still perform a successful upload, provided:

- Column fields are properly mapped within the worksheet
- Equivalent fields exist in ACA

Analysis Worksheet

On the Analysis worksheet, you will specify the Analysis ID to which you want link the Assets. The Analysis ID column that appears on this worksheet also appear on the Assets worksheet, and is used to identify the records that will be linked to the analysis.

Note: Each row in this worksheet represents a unique analysis. You should not include the same analysis more than once.

Field Caption	Field ID	Data Type (Length)	Comments
Analysis ID	MI_AN_ANALY_ID_CHR	Character (255)	This field is required and must be unique.
Site Reference Name	MI_SITE_NAME	Character (50)	This field is required and must match an existing Site name. Note: If you want to set the site reference to be a Global Site Reference, enter the constant *Global* in the MI_SITE_NAME column on the spreadsheet.
Analysis Description	MI_AN_SHORT_DESCR_CHR	Character(255)	This field contains a brief description about the Asset Criticality Analysis.

Asset Worksheet

On the Asset worksheet, you will specify the assets that will be created and linked to analysis.

Note: Each row in this worksheet represents a unique aAsset. You should not include the same asset more than once to the same analysis.

Note: When you enter N/A in the column for any of the Safety, Environment, Operations, or Financial values in the Data Loader, the associated Unmitigated Risk is set as Not Applicable.

Field Caption	Field ID	Data Type (Length)	Comments
Analysis ID	MI_AN_ANALY_ID_CHR	Character (255)	This field is required and must be unique.
Asset ID	ASSET_ID	Character (255)	This field displays the value that identifies the Asset.
Asset Family ID	ASSET_FAMILY	Character (255)	Based on the ID, this field is populates either an Equipment or a Functional Location.
Asset Field ID	ASSET_FIELD_ID	Character (30)	This field is the ID of the field that is used to identify the Asset.
(ENVIRONMENT) Consequence	ENVIRONMENT MI_CONSE_N	Numeric	Must be filled based on the risk matrix of the site.
(ENVIRONMENT) Probability	ENVIRONMENT MI_PROB_N	Numeric	Must be filled based on the risk matrix of the site.
(ENVIRONMENT) Protection Level	ENVIRONMENT MI_PROT_N	Numeric	Must be filled based on the risk matrix of the site.
(ENVIRONMENT) Risk Rank	ENVIRONMENT-RISK_RANK	Numeric	Must be filled based on the risk matrix of the site.

Field Caption	Field ID	Data Type (Length)	Comments
(FINANCIAL) Consequence	FINANCIAL MI_CONSE_N	Numeric	Must be filled based on the risk matrix of the site.
(FINANCIAL) Maintenance Cost	FINANCIAL MI_RISK_MAIN_COST_N	Numeric	Must be filled based on the risk matrix of the site.
(FINANCIAL) Probability	FINANCIAL MI_PROB_N	Numeric	Must be filled based on the risk matrix of the site.
(FINANCIAL) Production Loss	FINANCIAL MI_RISK_PROD_LOSS_N	Numeric	Must be filled based on the risk matrix of the site.
(FINANCIAL) Protection level	FINANCIAL MI_PROT_N	Numeric	Must be filled based on the risk matrix of the site.
(FINANCIAL) Risk Rank	FINANCIAL-RISK_RANK	Numeric	Must be filled based on the risk matrix of the site.
(OPERATIONS) consequence	OPERATIONS MI_CONSE_N	Numeric	Must be filled based on the risk matrix of the site.
(OPERATIONS) Probability	OPERATIONS MI_PROB_N	Numeric	Must be filled based on the risk matrix of the site.
(OPERATIONS) Protection Level	OPERATIONS MI_PROT_N	Numeric	Must be filled based on the risk matrix of the site.
(OPERATIONS) Risk Rank	OPERATIONS-RISK_RANK	Numeric	Must be filled based on the risk matrix of the site.
(SAFETY) Consequence	SAFETY MI_CONSE_N	Numeric	Must be filled based on the risk matrix of the site.
(SAFETY) Probability	SAFETY MI_PROB_N	Numeric	Must be filled based on the risk matrix of the site.
(SAFETY) Protection Level	SAFETY MI_PROT_N	Numeric	Must be filled based on the risk matrix of the site.
(SAFETY) Risk Rank	SAFETY-RISK_RANK	Numeric	Must be filled based on the risk matrix of the site.
Basis for Assesment	MI_RISKASSE_BASIS_T	Text	Must be filled based on the risk matrix of the site.

About the Asset Criticality Analysis (ACA) Data Loader Load Verification

About This Task

A successful data import will have the same effect as creating a new Asset Criticality Analysis in GE Digital APM. Following a successful data load, if the data loader created a new asset criticality analysis, it will appear in the Analyses section on the Asset Criticality Analysis Overview page.

A successful import can also be defined as an event in which partial data on a worksheet was loaded into GE Digital APM, and where the user was given appropriate messaging that enabled him or her to identify and correct issues resulting from the import.

Chapter 5

Deployment

Topics:

- [Deploy ACA for the First Time](#)
- [Upgrade or Update ACA to V4.4.0.0.0](#)
- [ACA Security Groups](#)

Deploy ACA for the First Time

Before You Begin

The following tables outline the steps that you must complete to upgrade this module to V4.4.0.0.0. These instructions assume that you have completed the steps for upgrading the basic GE Digital APM system architecture.

These tasks may be completed by multiple people in your organization. We recommend, however, that the tasks be completed in the order in which they are listed.

Results

Step	Task	Notes
1	Assign Security Users to one or more of the ACA Security Groups and Roles .	This step is required.
2	Review the ACA data model to determine which relationship definitions you will need to modify to include your custom equipment and location families. Via Configuration Manager, modify the relationship definitions as needed.	This step is required only if you store equipment and location information in families other than the baseline Equipment and Functional Location families.
3	Optional: Configure Criticality Definition records to use a Checklist as the Criticality Assessment method instead of the Risk Matrix.	To configure to use a Checklist, select the Use Checklist field and select the desired family from the Checklist Family field. To associate a Criticality Definition record with a Site, link the Criticality Definition record to a Site Reference record. The Criticality Checklist family datasheet and Before Insert Family Policy can be configured to implement the desired assessment input fields and criticality value calculation logic.

Upgrade or Update ACA to V4.4.0.0.0

Before You Begin

The following table outlines the steps that you must complete to deploy and configure this module for the first time. These instructions assume that you have completed the steps for deploying the basic system architecture.

These tasks may be completed by multiple people in your organization. GE Digital recommends, however, that the tasks be completed in the order in which they are listed.

Procedure

- Upgrade from any version V4.3.0.0.0 through V4.3.1.0.4

This module will be updated to V4.4.0.0 automatically when you update the components in the basic GE Digital APM system architecture. No additional steps are required.

- Upgrade from any version V4.2.0.0 through V4.2.0.9.4

Step	Task	Notes
1	Lock the Risk Matrix.	This step is required only if you do not want risk values to be specified manually via the Risk Matrix.
2	Create Criticality Mapping records and link them to corresponding Risk Threshold records.	This step is required only if you want to update your SAP system to reflect the criticality value that is determined in ACA.

- Upgrade from any version V4.1.0.0 through V4.1.7.4.0

Step	Task	Notes
1	Lock the Risk Matrix.	This step is required only if you do not want risk values to be specified manually via the Risk Matrix.
2	Create Criticality Mapping records and link them to corresponding Risk Threshold records.	This step is required only if you want to update your SAP system to reflect the criticality value that is determined in ACA.

- Upgrade from any version V4.0.0.0 through V4.0.1.0

Step	Task	Notes
1	Lock the Risk Matrix.	This step is required only if you do not want risk values to be specified manually via the Risk Matrix.
2	Create Criticality Mapping records and link them to corresponding Risk Threshold records.	This step is required only if you want to update your SAP system to reflect the criticality value that is determined in ACA.

- Upgrade from any version V3.6.1.0.0 through V3.6.1.7.4

Step	Task	Notes
1	Lock the Risk Matrix.	This step is required only if you do not want risk values to be specified manually via the Risk Matrix.
2	Create Criticality Mapping records and link them to corresponding Risk Threshold records.	This step is required only if you want to update your SAP system to reflect the criticality value that is determined in ACA.

- Upgrade from any version V3.6.0.0.0 through V3.6.0.12.9

Step	Task	Notes
1	Lock the Risk Matrix.	This step is required only if you do not want risk values to be specified manually via the Risk Matrix.
2	Create Criticality Mapping records and link them to corresponding Risk Threshold records.	This step is required only if you want to update your SAP system to reflect the criticality value that is determined in ACA.

- Upgrade from any version V3.5.1 through V3.5.1.12.3

Step	Task	Notes
1	Lock the Risk Matrix.	This step is required only if you do not want risk values to be specified manually via the Risk Matrix.
2	Create Criticality Mapping records and link them to corresponding Risk Threshold records.	This step is required only if you want to update your SAP system to reflect the criticality value that is determined in ACA.

- Upgrade from any version V3.5.0 SP1 LP through V3.5.0.1.10.1

Step	Task	Notes
1	Lock the Risk Matrix.	This step is required only if you do not want risk values to be specified manually via the Risk Matrix.
2	Create Criticality Mapping records and link them to corresponding Risk Threshold records.	This step is required only if you want to update your SAP system to reflect the criticality value that is determined in ACA.

- Upgrade from any version V3.5.0 through V3.5.0.0.7.1

Step	Task	Notes
1	Lock the Risk Matrix.	This step is required only if you do not want risk values to be specified manually via the Risk Matrix.
2	Create Criticality Mapping records and link them to corresponding Risk Threshold records.	This step is required only if you want to update your SAP system to reflect the criticality value that is determined in ACA.

- Upgrade from any version V3.4.5 through V3.4.5.0.1.4

Step	Task	Notes
1	Lock the Risk Matrix.	This step is required only if you do not want risk values to be specified manually via the Risk Matrix.
2	Create Criticality Mapping records and link them to corresponding Risk Threshold records.	This step is required only if you want to update your SAP system to reflect the criticality value that is determined in ACA.

- When upgrading to 4.3.0.7.0, all existing Asset Criticality Analysis Systems are now displayed in the list of Asset Criticality Analyses.

- When upgrading to 4.3.0.7.0, the Team Members and Reference Documents of existing Asset Criticality Analysis records will be transferred to the associated records in the Asset Criticality Analysis System family.
- When upgrading to 4.3.0.7.0, the State of existing Asset Criticality Analysis records will be transferred to the child records in the Asset Criticality Analysis System family. The States for Asset Criticality Analyses will be upgraded from:
 - Complete to Approved
 - Pending Approval to Pending Approval
 - All other States will be upgraded to In Progress
- When upgrading to 4.3.0.7.0, State Management roles need to be configured for the Asset Criticality Analysis System family.
- When upgrading to 4.3.0.7.0, corresponding Criticality Definition and Criticality Threshold records will be created from existing Risk Matrix records.

ACA Security Groups

The following table lists the baseline Security Groups available for users within this module, as well as the baseline Roles to which those Security Groups are assigned.

Important: Assigning a Security User to a Role grants that user the privileges associated with all of the Security Groups that are assigned to that Role. To avoid granting a Security User unintended privileges, before assigning a Security User to a Role, be sure to review all of the privileges associated with the Security Groups assigned to that Role. Also, be aware that additional Roles, as well as Security Groups assigned to existing Roles, can be added via Security Manager.

Security Group	Roles
MI ACA Administrator	MI Foundation Admin
MI ACA Member	MI Foundation Admin MI Foundation Power MI Foundation User MI APM Viewer
MI ACA Owner	MI Foundation Admin MI Foundation Power

The baseline family-level privileges that exist for these Security Groups are summarized in the following table.

Family	MI ACA Administrator	MI ACA Member	MI ACA Owner
Entity			
Asset Criticality Analysis	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Asset Criticality Analysis Has System	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Asset Criticality Analysis System	View, Update, Insert, Delete	View	View, Update, Insert, Delete

Family	MI ACA Administrator	MI ACA Member	MI ACA Owner
Consequence	View, Update, Insert, Delete	View	View
Consequence Modifier	View, Update, Insert, Delete	View	View
Criticality Mapping	View	View	View
Equipment	View	View	View
Functional Location	View	View	View
Analysis Has Human Resource	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Human Resource	View, Update, Insert, Delete	None	View, Update, Insert, Delete
General Recommendation	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Mitigates Risk	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Notification	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Probability	View, Update, Insert, Delete	View	View
Protection Level	View	View	View
RCM FMEA Analysis	View	None	None
Reference Document	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Risk	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Risk Assessment	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Risk Category	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Risk Matrix	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Risk Threshold	View, Update, Insert, Delete	View	View
Safety Analysis Has Equipment	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Site Reference	View	View	View
System Strategy	View	None	None
Relationship			
Equipment Has Equipment	View	View	View
Functional Location Has Equipment	View	View	View
Functional Location Has Functional Location	View	View	View
Has Criticality Mapping	View	View	View
Has Functional Location	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Has RCM FMEA Analysis	View	None	None
Has Recommendations	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Has Reference Documents	View, Update, Insert, Delete	View	View, Update, Insert, Delete

Family	MI ACA Administrator	MI ACA Member	MI ACA Owner
Has Reference Values	View, Update, Insert, Delete	View	View
Has Risk	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Has Risk Category	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Has Risk Matrix	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Has Site Reference	View, Update, Insert, Delete	View	View, Update, Insert, Delete
Has Strategy	View	None	None

Chapter 6

Reference

Topics:

- [General Reference](#)
- [Family Field Descriptions](#)
- [Catalog Items](#)

General Reference

ACA Data Model

An Asset Criticality Analysis (ACA) is composed of entity families, relationship families, and business rules. The workspaces in the ACA interface provide you with a custom view of ACA records that exist in the database.

The ACA Data Model uses families to represent the various [ACA records](#) and leverages the GE Digital APM fundamental entity and relationship family infrastructure to store data related to an ACA. The ACA interface is simply a customized view of individual records that make up an ACA.

All ACAs begin with an [ACA record](#). Each ACA record is linked to:

- One or more Human Resource records
- One or more Reference Document records

Each ACA System record is linked to:

- One or more assets
- One or more General Recommendation records


The ACA System family contains Asset Groups that are made up of Equipment and Functional Location records, and they can participate in additional relationships when integrated with modules within the Asset Strategy work process.

ACA Data Model

The following diagram illustrates the families that participate in an ACA.

The boxes represent entity families, and the arrows represent relationship families. You can determine the cardinality of a relationship from the direction of the arrow (for example, the arrow points to the successor family).

For example, ACA System records are linked to Risk Assessment records through the Has Risk relationship, where the ACA System family is the predecessor.

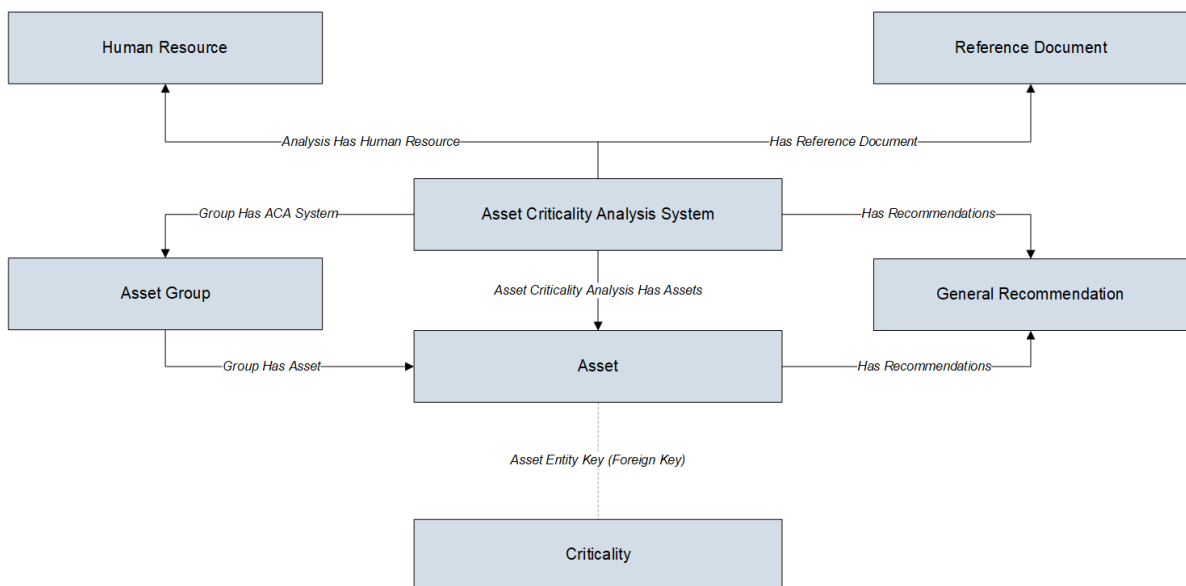

ACA Data Model Integrated with Asset Strategy

Depending on the licenses that have been activated in your database, you can promote records from ACA to the following modules in the Asset Strategy work process:

- Reliability Centered Maintenance (RCM)
- Failure Modes and Effects Analysis (FMEA)
- Asset Strategy Management (ASM)

Throughout the ACA documentation, we assume that the ASM, RCM, and FMEA modules are active.

The following diagrams illustrate the families that participate in the integration between ACA and RCM, FMEA, and ASM.

ACA URLs

There is one URL Route associated with accessing the Asset Criticality Analysis module: **aca**. The following table describes the various paths that build on the route, and the elements that you can specify for each.

Tip: For more information, refer to the URLs section of the documentation.

Element	Description	Accepted Value(s)	Notes
aca/overview: Opens the ACA Overview page.			
aca/analysis/<EntityKey>/<SectionName>: Opens a specific Asset Criticality analysis on the Analysis Summary page.			
<EntityKey>	Specifies the analysis that you want to view	Any Entity Key that corresponds to an analysis.	NA
		0	Opens a new analysis.
<SectionName>	Specifies the section in which you want to open the analysis.	definition	Opens the Analysis Definition section for the specific ACA.
		member	Opens the Team Members section for the specific ACA.

Example URLs


Example URL	Destination
aca/overview	The ACA Overview page
aca/analysis/123456	The Asset Criticality analysis with the Entity Key 123456.
aca/analysis/0/definition	The ACA Definition page for a new ACA record.
aca/analysis/<EntityKey>/member	The Team Members page for the ACA record identified with Entity Key 123456.

ACA State Configuration

States and Operations

The following diagram illustrates the baseline State Configuration workflow that is defined for the ACA family. The boxes represent states, and the arrows represent operations. You can determine the

cardinality of an operation from the direction of the arrow (that is, the state to which the arrow points is the successor state).

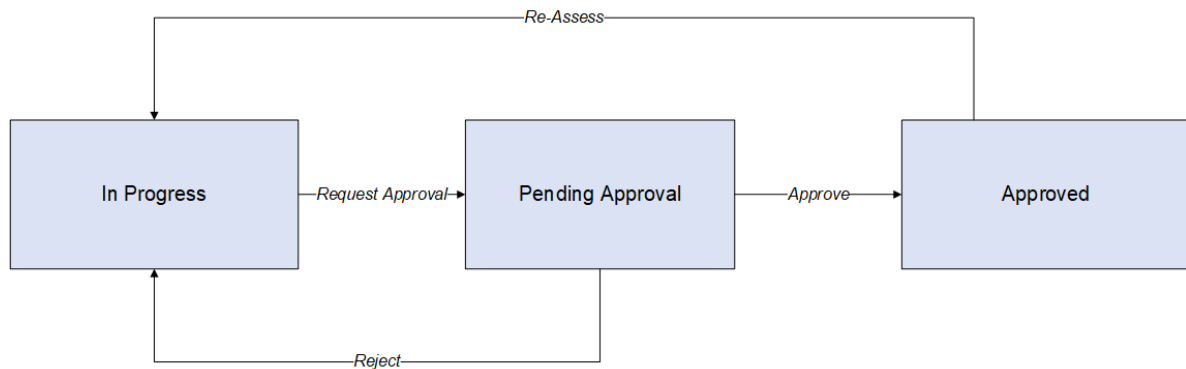

The following baseline State Configurations and operations exist for the ACA family:

- The Planning state is the initial state of all new ACA records.
- **Datasheet Configuration:** By default, states and operations will appear in the datasheet when you are viewing an ACA record.
- **Reserved States and Operations:** By default, all states and operations displayed in the diagram are reserved. This means that you cannot remove or modify any of these states or operations. You can, however, add your own states and operations to the State Configuration.
- **State Configuration Roles:** By default, the MI ACA Owner State Configuration Role is assigned to all predecessor and successor states in the ACA State Configuration. You can assign other State Configuration Roles to any state. In addition, for each state, the **Require a specific user to be assigned to a state** check box is selected.

The Approved state is the terminal state of all new ACA records.

- Once an analysis is in the Approved state, all functionalities will be disabled, except:
 - **Export**
 - **Send to Asset Strategy**
 - **Send to FMEA Analysis**
 - **Send to RBI Asset View**
 - **Send to RCM Analysis**
 - **Send to SAP**
 - **Send to System Strategy**

ACA Site Filtering

Tip: For more information, refer to the Site Filtering section of the documentation.

Site filtering in ACA is achieved by specifying a value in the Site Reference Key for a record. Users must have privileges for the relevant site to access records with a specified site. Users can be assigned to one or many sites. They will be able to view global data, as well as view data for each of the sites to which they are assigned.

Site filtering behavior is applied to all areas where data is handled in ACA including data loaders, asset hierarchy, global search, and queries throughout the ACA module.

In ACA, site filtering affects the following records:

- **ACA Record:** If an ACA record is assigned to the default site, only by users who have been assigned to the same site can access the record.
- **Asset Records:** The records are filtered and displayed based on the site value inherited from the user.

Important: A Super User can change the site to any of the sites that the user has permission for or choose to make the ACA record as a Global Record, so that all the GE Digital APM users can see it.

Family Field Descriptions

ACA Records

The following table provides an alphabetical list and description of the fields that exist in the ACA family. The information in the table reflects the baseline state and behavior of these fields.

This family is enabled for site filtering, which means that records in this family can be assigned to a specific site, and will then only be accessible to users who are assigned to the same site and have the appropriate license and family privileges. For more information, refer to the Sites section of the documentation.

Note: Only members of the MI ACA Administrator Security Group can modify the layout of the ACA datasheet.

Field	Data Type	Description	Behavior and Usage
Analysis Description	Character	A description of the ACA.	None
Analysis End Date	Date	The date on which the ACA will end.	None
Analysis ID	Character	The ID for the ACA.	This field is required, and the value must be unique.
Analysis Owner	Character	The name of the team member who is specified as the Process Owner for the ACA.	This field is disabled and populated automatically with the value in the Process Owner field.
Analysis Scope	Text	A description of the ACA that you want to conduct.	None
Analysis Start Date	Date	The date on which the ACA will begin.	None
Analysis Type	Character	N/A	By default, this field does not appear on the ACA datasheet.
Facilitator	Character	The name of the team member who is specified as the Facilitator for the ACA.	By default, this field does not appear on the ACA datasheet. This field is populated automatically with the name of the ACA team member specified as the Facilitator in the ACA Team Members section .

Field	Data Type	Description	Behavior and Usage
Imported By	Character	The user ID of the Security User who created or last updated the analysis from a Microsoft Excel file.	This field is disabled and populated automatically when you create an analysis or update the risk values by importing data from an Excel file.
Import Date	Date	The date on which the analysis was created or last updated from a Microsoft Excel file.	This field is disabled and populated automatically when you create an analysis or update the risk values by importing data from an Excel file.
Import Status	Character	The status of the import process that was last used to create or update the analysis.	<p>This field is disabled and populated automatically when you create an analysis or update the risk values by importing data from an Excel file.</p> <p>Tip: For more information, refer to the Data Loaders section of the documentation.</p> <p>The value will be set to one of the following:</p> <ul style="list-style-type: none"> • Successful • Incomplete • Failed • Skipped <p>The status is also displayed in the grid on the ACA Import page.</p>
Last Modified By	Character	The name of the user who last modified the record.	This field is disabled and populated automatically with the name of the user who was logged in when the record was last modified.
Last Modified Date	Date	The date on which the record was last modified.	This field is disabled and populated automatically.

Field	Data Type	Description	Behavior and Usage
Process Owner	Character	The name of the Process Owner for the ACA.	By default, this field does not appear on the ACA datasheet. It is populated automatically with the name of the ACA team member specified as the Process Owner in the ACA Team Members section. When a user creates a new ACA record, this value defaults to the name of the user who created the record. After a team member has been assigned to the role of Process Owner, this field will be updated automatically with that team member's name.
Visual Attributes	Text	N/A	By default, this field does not appear on the ACA datasheet.

Criticality Records

Criticality records store assessment data to allow future expanded criticality options and assessment features. This topic provides an alphabetical list and description of the fields that exist for the Criticality family. The information in the table reflects the baseline state and behavior of these fields.

Field	Data Type	Description	Behavior and Usage
Assessment	Text	Stores a serialized JSON representation of criticality that has been assessed using the Risk Matrix or Criticality Matrix tool.	This is a system field.
Assessment Method	Text	Describes how criticality was assessed.	A system field that contains one of the following values: <ul style="list-style-type: none"> Checklist Matrix
Asset Key	Numeric	The Entity Key of the asset.	None.
Basis for Assessment	Character	A brief summary of the rationale used to assess criticality.	This field is automatically populated with the value you enter in the Basis for Assessment field.
Threshold Key	Numeric	The numeric key indicating the label and color associated with the threshold value.	A numeric key that determines the label and color associated with the Criticality record. It is also a foreign key to the Criticality Threshold family.
Value	Numeric	Stores the canonical criticality value for a given asset.	The value in this field is used as the basis for computing the Criticality Definition threshold.

Criticality Checklist Records

This family is a template for assessing criticality with the Criticality Checklist. This topic provides an alphabetical list and description of the fields that exist for the Criticality family. The information in the table reflects the baseline state and behavior of these fields.

Field	Data Type	Description	Behavior and Usage
Basis for Assessment	Text	Provides details about the Criticality Assessment.	This field is automatically populated with the value you enter in the Basis for Assessment field.
Environment Consequence	Character	Assesses the environmental consequence of the Criticality Checklist item.	Populated automatically from the criticality value assessed from the environmental effects of an asset.
Operations Consequence	Character	Assesses the operations consequence of the Criticality Checklist item.	Populated automatically from the criticality value assessed from the operational effects of an asset.
PM Required	Boolean	Indicates whether or not preventive maintenance is required.	If the value in this field is true, then the asset requires preventive maintenance.
Safety Consequence	Character	Assesses the safety consequence of the Criticality Checklist item.	Populated automatically from the criticality value assessed from the safety effects of an asset.

Criticality Definition Records

Criticality Definition records store references to the criticality thresholds and assessment options. It also enables the user to modify assessment methods. This topic provides an alphabetical list and description of the fields that exist for the Criticality Definition family. The information in the table reflects the baseline state and behavior of these fields.

Field	Data Type	Description	Behavior and Usage
Checklist Family	Character	The family ID of the Criticality Checklist family used for assessment.	If the Use Checklist check box is selected, then the family indicated in this field will be required.
Default	Boolean	Indicates whether or not this is the default Criticality Definition.	You can specify only one Criticality Definition record as the default. In the Standard Practice Criticality Definition record, the Default check box is cleared. In the Default Criticality Definition record, the Default check box is selected.
Name	Character	The name of the Criticality Definition.	This value is used to identify the record and must be unique. In the baseline Criticality Definition record, the Criticality Definition name is Default.
Use Checklist	Boolean	Indicates whether or not to use the Criticality Checklist Assessment method.	If this check box is selected, then this will be used, and this will be required.

Criticality Threshold Records

Criticality Threshold records store the threshold bands that define a criticality definition. This topic provides an alphabetical list and description of the fields that exist for the Criticality Threshold family. The information in the table reflects the baseline state and behavior of these fields.

Field	Data Type	Description	Behavior and Usage
Color	Character	The color of the criticality badge.	None
Description	Character	The description of the criticality value.	None
Value	Numeric	A number that represents the threshold level associated with the criticality value.	This value is the lower limit for a given threshold.

Catalog Items

Catalog Folder Structure

The ACA Catalog folders contain dashboards, queries, graphs, and reports that appear throughout the ACA module and display information contained in the records that make up ACAs. The Catalog folder \

\\Public\Meridium\Modules\Asset Criticality Analysis contains the following subfolders:

- **Dashboards:** Contains the dashboard ACA Overview.
- **Graphs:** Contains the graph Asset Criticality Analysis Unmitigated Risk Graph and one subfolder, Subgraphs, which contains the supporting graphs for the ACA Unmitigated Risk Graph.
- **Queries:** Contains queries that are used by ACA to display information such as the list of existing ACA records and to support the reports stored in the folder \\Public\Meridium\Modules\Asset Criticality Analysis\Reports.
- **Reports:** Contains the report Asset Criticality Analysis Report and one subfolder, Subreports, which contains the supporting subreports for the ACA Report.

The topics in this section of the Help system describe the content of each Catalog folder in this list. You should not modify the names of these Catalog folders or the names of the items that exist in these folders or move the items to another Catalog folder.

Dashboards Folder

The dashboard listed in the following table is provided in the Catalog folder \\Public\Meridium\Modules\Asset Criticality Analysis\Dashboards. In the following table, the value listed in the Dashboard column refers to the dashboard name.

Dashboard	Behavior and Usage
ACA Overview	Displays the ACA Overview page, which features graphs representing the ACAs according to their state and the Asset Criticality Distribution, as well as links to the individual ACAs.

Graphs Folder

The graph listed in the following table is provided in the Catalog folder \\Public\Meridium\Modules\Asset Criticality Analysis\Graphs. In the following table, the value listed in the Graph column refers to the graph name.

Graph	Behavior and Usage
ACA Analyses by State	Displayed on the ACA Overview page.
Asset Criticality Distribution	Displayed on the ACA Overview page.

The Subgraphs folder is a level below the Graphs folder in the Catalog folder \\Public\Meridium\Modules\Asset Criticality Analysis\Subgraphs. The following table gives the names of the subgraphs as well as their use.

Subgraph	Behavior and Usage
ACA Equipment Lists	Supports Asset Criticality Analysis Unmitigated Risk Graph.
ACA Location Equipment Unmitigated Risk	Supports Asset Criticality Analysis Unmitigated Risk Graph.

Important: Graphs that you are unable to view in GE Digital APM are viewable in the **Catalog** folder.

Queries Folder

The queries listed in the following table are provided in the Catalog folder \\Public\Meridium\Modules\Asset Criticality Analysis\Queries. In this table, the values listed in the Query column refer to the query names. The baseline captions are the same as the names.

Query	Behavior and Usage
ACA	After displaying a prompt for an Entity Key, returns the Asset Criticality Analysis record with the specified Entity Key. This query supports the report Asset Criticality Analysis Report, which is stored in the Reports folder.
ACA All Assets	After displaying a prompt for an Entity Key, returns the assets that are defined in the specified Asset Hierarchy. The results of this query appear when you access the Assets section in the Asset Criticality Overview page.
ACA Analysis Assets	After displaying a prompt for an analysis key, displays a list of assets in the analysis.
ACA Analysis Criticality	After displaying a prompt for a criticality value, returns the assessed criticality value linked to the Asset Criticality Analysis record. The results of this query appear when a Risk Assessment has completed.
ACA Recommendations	After displaying a prompt for an Entity Key, returns the General Recommendation records that are linked to the Asset Criticality Analysis record with the specified Entity Key. The results of this query appear when you select the ACA Recommendations page.
ACA Reference Document Query	After displaying a prompt for an Entity Key, returns the Reference Document records that are linked to the Asset Criticality Analysis record with the specified Entity Key. This query supports the report Asset Criticality Analysis Report that is stored in the Reports folder.
ACA Search	After displaying a prompt for a state value, returns the Asset Criticality Analysis records that are set to the specified state. The results of this query appear when you access the ACA Search page.

Query	Behavior and Usage
ACA System Search	Displaying a prompt for an Analysis Key and ID, where the Analysis Key is the Analysis Key for an Asset Criticality Analysis record and ID is the System ID of an Asset Criticality Analysis System record. The query returns the Asset Criticality Analysis System record with the specified ID that is linked to the Asset Criticality Analysis record with the specified Analysis Key. The results of this query appear when you access the ACA System page.
ACA Team Member Query	After displaying a prompt for an Entity Key, returns the Human Resource records that are linked to the Asset Criticality Analysis record with the specified Entity Key. This query supports the report Asset Criticality Analysis Report stored in the Reports folder.

Reports Folder

The report listed in the following table is provided in the Catalog folder `\\Public\Meridium\Modules\Asset Criticality Analysis\Reports`. In this table, the values listed in the Report column refer to the report name. The baseline caption is the same as the name.

Report	Behavior and Usage
ACA Report	After displaying a prompt for an Entity Key, displays a summary of the information related to the Asset Criticality Analysis record with the specified Entity Key.

The reports listed in the following table are provided in the Catalog folder `\\Public\Meridium\Modules\Asset Criticality Analysis\Reports\Subreports`. In this table, the values listed in the Report column refer to the report names. The baseline captions are the same as the names.

Report	Behavior and Usage
ACA Reference Documents Report	After displaying a prompt for an Entity Key, displays the Reference Document records that are linked to the Asset Criticality Analysis record with the specified Entity Key.
ACA System Lists Report	After displaying a prompt for an Entity Key, displays the Asset Criticality Analysis System records that are linked to the Asset Criticality Analysis record with the specified Entity Key.
ACA Team Members Report	After displaying a prompt for an Entity Key, displays the list of team members whose Human Resource record is linked to the Asset Criticality Analysis record with the specified Entity Key.